



# CERTIFICATE OF ACCREDITATION

**The ANSI National Accreditation Board**

Hereby attests that

**Keysight Technologies, Inc.**  
**10090 Foothills Blvd.**  
**Roseville, CA 95747**  
**(and satellite sites as listed on the scope)**

Fulfills the requirements of

**ISO/IEC 17025:2017**

and national standards

**ANSI/NCSL Z540-1-1994 (R2002) and**  
**ANSI/NCSL Z540.3-2006 (R2013)**

In the field of

**CALIBRATION**

This certificate is valid only when accompanied by a current scope of accreditation document.  
The current scope of accreditation can be verified at [www.anab.org](http://www.anab.org).

Jason Stine, Vice President

Expiry Date: 16 November 2026  
Certificate Number: AC-1498



This laboratory is accredited in accordance with the recognized International Standard ISO/IEC 17025:2017.  
This accreditation demonstrates technical competence for a defined scope and the operation of a laboratory  
quality management system (refer to joint ISO-ILAC-IAF Communiqué dated April 2017).

**SCOPE OF ACCREDITATION TO ISO/IEC 17025:2017**

**AND**

**ANSI/NCSL Z540-1-1994 (R2002)**

**ANSI/NCSL Z540.3-2006 (R2013)**

**Keysight Technologies, Inc.**

10090 Foothills Blvd.  
Roseville, CA 95747

Mr. Chris Cox +1 (916) 788-5594 [chris\\_cox@keysight.com](mailto:chris_cox@keysight.com)  
Ms. Bee-Choo Lim +65 6215 7191 [bee-choo\\_lim@keysight.com](mailto:bee-choo_lim@keysight.com)

**CALIBRATION**

ISO/IEC 17025 Accreditation Granted: **16 November 2024**

Certificate Number: **AC-1498** Certificate Expiry Date: **16 November 2026**

**Services performed at satellite laboratories for the main scope**

Customers submitting items to Keysight for calibration will be directed to the appropriate delivery site based on capability, geography and capacity.

Calibration and Measurement Capabilities (CMC) are available at each site. The lowest uncertainties are achieved at the Roseville location. Calibrations are performed at the most suitable site based on customer needs and location and the resultant uncertainties may be higher based on equipment performance.

Site Name	Site Address
Tempe, AZ	1829 West Drake Drive, Suite 101 Tempe, AZ 85283
Plantation, FL	8000 W. Sunrise Boulevard Plantation, FL 33322
Fort Wayne, IN	1200 Airport North Office Park, Unit C/D Fort Wayne, IN 46825
Nashua, NH	22 Cotton Road, Suite 150 Nashua, NH 03063
Greensboro, NC	7907 Piedmont Triad Parkway Greensboro, NC 27409
Bethlehem, PA	2840 Emrick Blvd., Suite A-4 Bethlehem, PA 18020
Richardson, TX	1220 E. Campbell Road Richardson, TX 75081
West Valley City, UT	2550 South Decker Lake Blvd., Suite #3 West Valley City, UT 84119



**ANSI National Accreditation Board**

Site Name	Site Address
Redmond, WA	4729 154 <sup>th</sup> Place NE, Building 87, Room 1437 Redmond, WA 98052
Brazil	Avenida Marcos Penteadado de Ulhoa Rodrigues, 939-6 <sup>o</sup> andar Barueri, SP, Brazil
Montreal, Canada	2250 Boul. Alfred Nobel, St. Laurent, Ste 102 Montreal, QC Canada H4S 2C9
Calgary, Canada	4720 14 St N.E. Calgary, AB T2E 6L7, Canada
Ottawa, Canada	350 Terry Fox Drive, Suite 106 Ottawa, ON, Canada K2K 2W5
Mexico	Av. Camino Al ITESO 8900-1B, Col Technological Industrial Park Tlaquepaque, Jalisco, 45609, Mexico
Japan	9-1 Takakura-Cho, Hachioji-shi Tokyo, 192-8550 Japan
South Korea	Singsong Center Bldg. 15F, #57, Yeouinaru-ro, Yeongdeungpo-gu, Seoul, Korea
Singapore	1 Yishun Avenue 7 Singapore 768923
Vietnam	6th Floor, Lot 601, CMC Tower, 11 Duy Tan Alley Cau Giay Ward, Hanoi, Vietnam
India	The Millenia, Second floor, Tower 'D', No. 1&2 Murphy Road, Ulsoor, Bangalore, Karnataka, 560 008, India
Taiwan	No. 20, Kao-Shuang Road Ping-Chen district 32450, Tao-Yuan City, Taiwan R.O.C.
Beijing, China	No.3 Wang Jing Bei Lu Chao Yang District, Beijing, China
Chengdu, China	Chengdu Hi-Tech Industrial Development Zone (South) No. 116 Tian Fu 4th Street, Chengdu, China
Malaysia	Phase 3 Bayan Lepas Free Industrial Zone 11900 Bayan Lepas, Penang, Malaysia

**Services performed at satellite laboratories with unique scopes**

Site Name	Site Address
<a href="#">El Segundo, CA</a>	700 Lairport Street El Segundo, CA 90245
<a href="#">Kimballton, IA</a>	1346 Yellowwood Road Kimballton, IA 51543
<a href="#">Elk Horn, IA</a>	2012 High Street Elk Horn, IA 51531

## Services performed at main laboratory and satellite locations

### Electrical – DC/Low Frequency

### Main Scope

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
DC Ratio <sup>1</sup>	(>0 to 10) V	$1.7 \times 10^{-8}$	Comparison to a DC voltage standard
DC Voltage – Source	(>0 to 10) V	1.1 nV	Comparison to a programmable Josephson voltage standard
DC Voltage – Source	(>0 to 220) mV (0.22 to 2.2) V (2.2 to 11) V (11 to 22) V (22 to 220) V (220 V to 1 100) V	$7 \mu\text{V/V} + 0.39 \mu\text{V}$ $4.7 \mu\text{V/V} + 0.62 \mu\text{V}$ $3.1 \mu\text{V/V} + 2.3 \mu\text{V}$ $3.1 \mu\text{V/V} + 4.2 \mu\text{V}$ $4.7 \mu\text{V/V} + 39 \mu\text{V}$ $6.2 \mu\text{V/V} + 0.39 \text{mV}$	Direct comparison to a DC voltage standard
DC Voltage – Source	0 V (>0 to 0.1) V (0.1 to 1) V (1 to 10) V (10 to 100) V (100 to 1 000) V	20 nV $0.24 \mu\text{V/V}$ $0.057 \mu\text{V/V}$ $0.027 \mu\text{V/V}$ $0.14 \mu\text{V/V}$ $0.16 \mu\text{V/V}$	Comparison to a DC voltage standard and a resistive divider
DC Voltage – Measure	(>0 to 10) V	5.5 nV	Comparison to a programmable Josephson voltage standard
DC Voltage – Measure	(>0 to 0.1) V (0.1 to 1) V (1 to 10) V (10 to 100) V (100 to 1 000) V	$4.1 \mu\text{V/V} + 0.36 \mu\text{V}$ $3.7 \mu\text{V/V} + 0.35 \mu\text{V}$ $3.1 \mu\text{V/V} + 0.59 \mu\text{V}$ $5.3 \mu\text{V/V} + 36 \mu\text{V}$ $5.3 \mu\text{V/V} + 0.12 \text{mV}$	Direct measurement with a Keysight 3458A multimeter
DC Voltage – Measure	(0.25 to 3) kV (3 to 5) kV	110 $\mu\text{V/V}$ 120 $\mu\text{V/V}$	Comparison to a Keysight 3458A multimeter and a high voltage divider
DC Voltage – Measure (Differential)	(>0 to 0.1) V (0.1 to 1) V (1 to 10) V (10 to 100) V (100 to 1 000) V	$0.61 \mu\text{V/V} + 0.061 \mu\text{V}$ $0.37 \mu\text{V/V} + 0.12 \mu\text{V}$ $0.061 \mu\text{V/V} + 0.61 \mu\text{V}$ $0.61 \mu\text{V/V} + 0.012 \text{mV}$ $1.8 \mu\text{V/V} + 0.061 \text{mV}$	Differential measurement with a Keysight 3458A multimeter

**Electrical – DC/Low Frequency**

**Main Scope**

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
DC Current – Source & Measure	0 A (>0 to 100) nA 100 nA to 1 $\mu$ A (1 to 10) $\mu$ A (10 to 100) $\mu$ A 100 $\mu$ A to 1 mA (1 to 10) mA (10 to 100) mA (0.1 to 1) A (1 to 10) A (10 to 20) A	42 pA 1.2 $\mu$ A/A 1.1 $\mu$ A/A 1.2 $\mu$ A/A 0.2 $\mu$ A/A 0.26 $\mu$ A/A 0.23 $\mu$ A/A 0.2 $\mu$ A/A 1 $\mu$ A/A 3.5 $\mu$ A/A 19 $\mu$ A/A	Comparison to reference resistors and a multimeter
DC Current – Source	(>0 to 220) $\mu$ A (0.22 to 2.2) mA (2.2 to 22) mA (22 to 100) mA (100 to 200) mA (0.22 to 1) A (1 to 1.6) A (1.6 to 2.2) A (2.2 to 11) A (11 to 20.5) A	39 $\mu$ A/A + 5.4 nA 31 $\mu$ A/A + 6.3 nA 31 $\mu$ A/A + 39 nA 39 $\mu$ A/A + 0.62 $\mu$ A 52 $\mu$ A/A - 0.74 $\mu$ A 70 $\mu$ A/A + 12 $\mu$ A 110 $\mu$ A/A - 21 $\mu$ A 150 $\mu$ A/A - 92 $\mu$ A 280 $\mu$ A/A + 370 $\mu$ A 0.82 mA/A + 0.89 $\mu$ A	Comparison to a DC current source
DC Current – Source	(10 to 1 025) A	0.2 % of reading	Comparison to DC current source and current coil
DC Current – Measure	0 pA (0.1 to 1.15) pA (1 to 115) pA (10 to 115) pA (0.1 to 1.15) nA (1 to 11.5) nA (10 to 115) nA (0.1 to 1.15) $\mu$ A (1 to 11.5) $\mu$ A	0.49 fA 0.83 mA/A + 0.59 fA 0.92 mA/A + 0.38 fA 0.24 mA/A + 1.4 fA 0.24 mA/A + 21 fA 26 $\mu$ A/A + 0.25 pA 51 $\mu$ A/A + 0.54 pA 20 $\mu$ A/A + 1.7 pA 13 $\mu$ A/A + 28 pA	Comparison to a Keysight 3458A multimeter and reference resistors

**Electrical – DC/Low Frequency**

**Main Scope**

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
DC Current – Measure	(0 to 100) nA (0.1 to 1) $\mu$ A (1 to 10) $\mu$ A (10 to 100) $\mu$ A (0.1 to 1) mA (1 to 10) mA (10 to 100) mA (0.1 to 1) A (1 to 3) A	42 $\mu$ A/A + 50 pA 21 $\mu$ A/A + 50 pA 25 $\mu$ A/A + 0.11 nA 25 $\mu$ A/A + 0.85 nA 22 $\mu$ A/A + 6.4 nA 23 $\mu$ A/A + 59 nA 41 $\mu$ A/A + 0.6 $\mu$ A 125 $\mu$ A/A + 12 $\mu$ A 1.4 mA/A + 0.74 mA	Direct measurement with a Keysight multimeter
DC Current – Measure	(0.10 to 1) A (1 to 100) A (100 to 500) A (500 to 1 000) A	73 $\mu$ A/A + 1.3 $\mu$ A 74 $\mu$ A/A - 0.021 $\mu$ A 58 $\mu$ A/A + 180 $\mu$ A 140 $\mu$ A/A + 0.42 mA	Comparison to a DC current shunt and a Keysight 3458A multimeter
DC Current – Measure	(5 to 10) A (10 to 30) A (30 to 36) A (36 to 45) A (45 to 60) A (60 to 90) A (90 to 180) A (180 to 340) A (340 to 510) A (510 to 1 000) A (1 000 to 2 000) A	93 $\mu$ A/A + 0.39 mA 140 $\mu$ A/A 94 $\mu$ A/A + 1.5 mA 92 $\mu$ A/A + 1.9 mA 93 $\mu$ A/A + 2.6 mA 91 $\mu$ A/A + 4 mA 87 $\mu$ A/A + 8.5 mA 200 $\mu$ A/A 180 $\mu$ A/A + 8.8 mA 180 $\mu$ A/A + 18 mA 150 $\mu$ A/A + 26 mA	Comparison to a DC current transducer and a Keysight 3458A multimeter
DC Current – Measure (Differential)	10 $\mu$ A to 100 $\mu$ A 100 $\mu$ A to 1 mA	24 $\mu$ A/A + 0.97 nA 24 $\mu$ A/A + 6.1 nA	Differential measurement with a multimeter
DC Current – Measure (Differential)	1 mA to 10 mA 10 mA to 100 mA 100 mA to 1.0 A 1 A to 10 A 10 A to 30 A 30 A to 50 A 50 A to 100 A 100 A to 300 A 300 A to 500 A 500 A to 1 000 A	0.61 $\mu$ A/A + 6.1 nA 0.061 $\mu$ A/A + 6 nA 0.061 $\mu$ A/A + 61 nA 0.061 $\mu$ A/A + 1 $\mu$ A 0.061 $\mu$ A/A + 6.1 $\mu$ A 0.061 $\mu$ A/A + 12 $\mu$ A 0.37 $\mu$ A/A + 12 $\mu$ A 0.37 $\mu$ A/A + 0.12 mA 0.37 $\mu$ A/A + 0.24 mA 0.61 $\mu$ A/A + 0.61 mA	Differential measurement with a multimeter and a resistive shunt
AC Ratio - Measure <sup>1</sup>	400 Hz to 1 kHz 0.1 to 1 Ratio	3 x 10 <sup>-7</sup>	Comparison to a ratio transformer

**Electrical – DC/Low Frequency**

**Main Scope**

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
AC DC Difference - Measure	(0.5, 1, 3 ,6) V		Comparison to an AC DC transfer standard
	3 MHz	0.11 mV/V	
	8 MHz	0.32 mV/V	
	10 MHz	0.35 mV/V	
	20 MHz	0.58 mV/V	
	30 MHz	0.73 mV/V	
	50 MHz	1.6 mV/V	
	70 MHz	2.8 mV/V	
	80 MHz	3 mV/V	
100 MHz	3.6 mV/V		
AC Current – Source (Relative) <sup>1</sup>	100 kHz to 100 MHz Ratio 0.7 to 1.1	0.058	Comparison to an oscilloscope
AC Current – Source	1 kHz		Comparison to a multifunction calibrator and a Keysight 3458A multimeter
	10 μA	3 nA	
	100 μA	2.5 nA	
	1 mA	32 nA	
	10 mA	330 nA	
	100 mA	3.3 μA	
1 A	38 μA		
AC Current - Measure	(45 to 100) Hz		Comparison to an AC current transducer and a Keysight 3458A multimeter
	(5 to 10) A	0.82 mA/A + 1.5 mA	
	(10 to 60) A	1 mA/A	
	(90 to 90) A	0.78 mA/A + 18 mA	
	(90 to 180) A	0.78 mA/A + 37 mA	
	(180 to 240) A	1 mA/A + 0.12 A	
	(240 to 360) A	1 mA/A + 0.18 A	
(360 to 700) A	1 mA/A + 0.36 A		
DC Resistance – Source	1 Ω	86 μΩ/Ω	Comparison to a multifunction calibrator
	1.9 Ω	85 μΩ/Ω	
	(10, 19) Ω	21 μΩ/Ω	
	(100, 190) Ω	9.3 μΩ/Ω	
	(1, 1.9, 10, 19) kΩ	6.2 μΩ/Ω	
	100 kΩ	7.8 μΩ/Ω	
	190 kΩ	9.3 μΩ/Ω	
	1 MΩ	12 μΩ/Ω	
	1.9 MΩ	16 μΩ/Ω	
	10 MΩ	36 μΩ/Ω	
	19 MΩ	43 μΩ/Ω	
	100 MΩ	93 μΩ/Ω	

**Electrical – DC/Low Frequency**

**Main Scope**

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
DC Resistance – Source	(>0 to 11) Ω (11 to 110) Ω (0.11 to 1.1) kΩ (1.1 to 3.3) kΩ (3.3 to 11) kΩ (11 to 110) kΩ 110 kΩ to 1.1 MΩ (1.1 to 3.3) MΩ (3.3 to 11) MΩ (11 to 33) MΩ (33 to 110) MΩ (110 to 330) MΩ (330 to 1 100) MΩ	33 μΩ/Ω + 8.3 mΩ 25 μΩ/Ω + 12.5 mΩ 23 μΩ/Ω + 17 mΩ 23 μΩ/Ω + 170 mΩ 23 μΩ/Ω + 84 mΩ 23 μΩ/Ω + 0.84 Ω 27 μΩ/Ω + 8 Ω 50 μΩ/Ω + 125 Ω 110 μΩ/Ω + 0.2 kΩ 210 μΩ/Ω + 2 kΩ 410 μΩ/Ω + 2.8 kΩ 2.5 mΩ/Ω + 83 kΩ 12 mΩ/Ω + 0.4 MΩ	Comparison to a multiproduct calibrator
DC Resistance – Source and Measure	Short (>0 to 100) mΩ 100 mΩ to 10 Ω (10 to 100) Ω 100 Ω to 1 kΩ (1 to 10) kΩ (10 to 100) kΩ 100 kΩ to 1 MΩ (1 to 10) MΩ (10 to 100) MΩ 1 GΩ 10 GΩ 100 GΩ	0.02 μΩ 0.064 μΩ/Ω 0.065 μΩ/Ω 0.082 μΩ/Ω 0.096 μΩ/Ω 0.095 μΩ/Ω 0.17 μΩ/Ω 0.35 μΩ/Ω 0.69 μΩ/Ω 4.1 μΩ/Ω 41 μΩ/Ω 46 μΩ/Ω 52 μΩ/Ω	Comparison to reference resistors, a resistance bridge and a high resistance meter
DC Resistance – Source and Measure	0 Ω 10 Ω 100 Ω 1 kΩ 10 kΩ 100 kΩ 1 MΩ 10 MΩ 100 MΩ	7.6 μΩ 13 μΩ 76 μΩ 0.40 mΩ 4.5 mΩ 42 mΩ 0.88 Ω 22 Ω 1.3 kΩ	Comparison to a multifunction calibrator and a Keysight 3458A multimeter

**Electrical – DC/Low Frequency**

**Main Scope**

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
DC Resistance - Measure	(0 to 12) Ω (12 to 100) Ω (0.1 to 1.2) kΩ (1.2 to 12) kΩ (12 to 120) kΩ (0.12 to 1.2) MΩ (1.2 to 12) MΩ (12 to 120) MΩ (0.12 to 1.2) GΩ	20 μΩ/Ω + 79 μΩ 15 μΩ/Ω + 0.79 mΩ 13 μΩ/Ω + 0.79 mΩ 13 μΩ/Ω + 7.8 mΩ 13 μΩ/Ω + 78 mΩ 17 μΩ/Ω + 2.6 Ω 61 μΩ/Ω + 0.12 kΩ 0.58 mΩ/Ω + 3.6 kΩ 5.7 mΩ/Ω + 0.26 MΩ	Comparison to a Keysight 3458A multimeter
Capacitance – Source	(0.19 to 3.29) nF (3.3 to 10.99) nF (11 to 109.99) nF (110 to 329.99) nF (0.33 to 1.099) μF (1.1 to 3.299) μF (3.3 to 10.99) μF (11 to 32.99) μF (33 to 109.99) μF (110 to 329.99) μF (0.33 to 1.099) mF (1.1 to 3.299) mF (3.3 to 10.00) mF (11 to 32.99) mF (33 to 110) mF	3.1 mF/F + 7.7 pF 1.4 mF/F + 8.2 pF 1.4 mF/F + 80 pF 1.5 mF/F + 0.24 nF 1.4 mF/F + 0.82 nF 1.5 mF/F + 2.4 nF 1.4 mF/F + 8.1 nF 2.4 mF/F + 24 nF 2.6 mF/F + 83 nF 2.7 mF/F + 0.24 μF 2.6 mF/F + 0.82 μF 2.7 mF/F + 2.4 μF 3.3 mF/F + 5.2 μF 5.5 mF/F + 24 μF 7.9 mF/F + 79 μF	Comparison to a multiproduct calibrator
Capacitance – Source	1 kHz 1 pF 10 pF 100 pF 1 nF 10 nF 100 nF 1 μF	11 μF/F 5.4 μF/F 1.9 μF/F 8.8 μF/F 27 μF/F 34 μF/F 43 μF/F	Comparison to reference capacitors and a ratio transformer

**Electrical – DC/Low Frequency**

**Main Scope**

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Capacitance - Measure	DC		Comparison to an LCR meter, DC current source and a Keysight 3458A multimeter
	0.2 mF	48 nF	
	0.3 mF	59 nF	
	0.33 mF	61 nF	
	0.7 mF	0.11 μF	
	1.09 mF	0.16 μF	
	1.1 mF	0.16 μF	
	2 mF	0.29 μF	
	3 mF	0.43 μF	
	3.3 mF	0.44 μF	
	10.9 mF	1.6 μF	
	20 mF	2.7 μF	
	30 mF	4.1 μF	
	33 mF	4.5 μF	
	110 mF	16 μF	
	(50, 100) Hz, 1 kHz		
	(0.19 to 1.2) nF	0.98 mF/F + 0.12 pF	
	(2 to 12) nF	0.9 mF/F + 0.23 pF	
	(20 to 120) nF	0.91 mF/F + 0.88 pF	
	(0.2 to 1.09) μF	0.91 mF/F + 8.1 pF	
(2 to 12) μF	0.91 mF/F + 95 pF		
20 μF	20 nF		
30 μF	30 nF		
33 μF	51 nF		
70 μF	120 nF		
109 μF	250 nF		
0.12 mF	280 nF		
Capacitance - Measure	1 kHz		Comparison to a capacitance bridge
	1 pF to 40 nF	3 μF/F	
	(40 to 100) nF	4 μF/F	
	(100 to 400) nF	5 μF/F	
	400 nF to 1.2 μF	8 μF/F	
Charge - Measure	DC		Comparison to reference capacitors and a Keysight 3458A multimeter
	(0 to 0.2) nC	0.079 pC	
	(0.2 to 2.0) nC	0.78 pC	
	(2 to 20) nC	4.5 pC	
	(20 to 200) nC	0.043 nC	
	(0.2 to 2) μC	0.43 nC	

**Electrical – DC/Low Frequency**

**Main Scope**

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Dissipation Factor – Measure <sup>1</sup>	>0 to 1 1 kHz 1 pF to 1 nF (1 to 10) nF (10 to 40) nF (40 to 70) nF (70 to 100) nF (100 to 200) nF (200 to 300) nF (300 to 400) nF (400 to 500) nF (500 to 600) nF (600 to 700) nF (700 to 800) nF (800 to 900) nF 900 nF to 1 μF (1 to 1.2) μF	0.000 003 0.000 005 0.000 01 0.000 015 0.000 02 0.000 04 0.000 055 0.000 075 0.000 095 0.000 11 0.000 13 0.000 15 0.000 16 0.000 18 0.000 21	Comparison to a capacitance bridge
Inductance – Measure	1 MHz 0.1 Ω 1 Ω 10 Ω 100 Ω	1 nH 0.3 nH 1 nH 7 nH	Comparison to a reference RL standard and an LCR Meter
Reactance – Measure	10 Ω 1 MHz (2, 3) MHz 4 MHz 5 MHz 10 MHz 13 MHz 100 Ω (1, 2, 3, 4, 5) MHz 10 MHz 13 MHz	4 mΩ 5 mΩ 6 mΩ 7 mΩ 20 mΩ 40 mΩ 40 mΩ 80 mΩ 90 mΩ	Comparison to reference RL, capacitance standards and an LCR Meter

**Electrical – DC/Low Frequency**

**Main Scope**

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Susceptance – Measure	1 kΩ		Comparison to reference RL, capacitance standards and an LCR Meter
	100 kHz	0.4 μS	
	(1, 2, 3, 4, 5) MHz	0.4 μS	
10 kΩ	0.7 μS		
(0.1, 1) MHz	0.04 μS		
100 kΩ	4 nS		
Temperature – Source <sup>3</sup> (simulation)	(-200 to -150) °C	$1.33 \times 10^{-5} T + 0.0036$ °C	Comparison to fixed resistors
	(-150 to 0) °C	$1.5 \times 10^{-5} T + 0.0038$ °C	
	(0 to 51.6) °C	$1.6 \times 10^{-5} T + 0.0038$ °C	
	(51.6 to 200) °C	$1.6 \times 10^{-5} T + 0.0053$ °C	
	(200 to 525) °C	$1.7 \times 10^{-5} T + 0.0051$ °C	
	(525 to 600) °C	$1.9 \times 10^{-5} T + 0.0041$ °C	
Temperature – Source (stimulation)	(-210 to -200) °C	0.22 °C	Comparison to a resistance or voltage generator
	(-200 to 0) °C	0.039 °C	
	(0 to 100) °C	0.055 °C	
	(100 to 300) °C	0.07 °C	
	(300 to 400) °C	0.078 °C	
	(400 to 630) °C	0.093 °C	
	(630 to 760) °C	0.14 °C	
	(760 to 800) °C	0.18 °C	
	(800 to 1 200) °C	0.19 °C	
	(1 200 to 1 372) °C	0.32 °C	

**Electrical – DC/Low Frequency**

**Main Scope**

Parameter/Equipment	AC DC Difference - Measure											
Reference Standard, Method, and/or Equipment	Comparison to an AC DC transfer standard											
Expanded Uncertainty of Measurement (+/-)												
Range	0.5 V	1 V	3 V	6 V	10 V	20 V	100 V	300 V	500 V	700 V	1000 V	
10 Hz	15 μV/V	6.3 μV/V	8.2 μV/V	57 μV/V	8.2 μV/V	-	6.9 μV/V	-	-	-	-	
20 Hz	11 μV/V	4.5 μV/V	-	-	5.1 μV/V	-	7.6 μV/V	-	-	-	-	
40 Hz	11 μV/V	3.8 μV/V	-	--	3.9 μV/V	-	6.3 μV/V	6.3 μV/V	9.2 μV/V	10 μV/V	10 μV/V	
100 Hz	12 μV/V	2.7 μV/V	3.1 μV/V	25 μV/V	3.1 μV/V	-	6.8 μV/V	6.4 μV/V	9.2 μV/V	9.3 μV/V	10 μV/V	
1 kHz	4.6 μV/V	3.1 μV/V	3.1 μV/V	2.9 μV/V	3.4 μV/V	3.5 μV/V	4 μV/V	6.6 μV/V	9.2 μV/V	9.9 μV/V	10 μV/V	

**Electrical – DC/Low Frequency**

**Main Scope**

Parameter/Equipment		AC DC Difference - Measure										
Reference Standard, Method, and/or Equipment		Comparison to an AC DC transfer standard										
Expanded Uncertainty of Measurement (+/-)												
Range	0.5 V	1 V	3 V	6 V	10 V	20 V	100 V	300 V	500 V	700 V	1000 V	
10 kHz	6 μV/V	3.5 μV/V	3.5 μV/V	34 μV/V	3 μV/V	-	4.3 μV/V	6.9 μV/V	9.4 μV/V	10 μV/V	11 μV/V	
20 kHz	7.4 μV/V	3.5 μV/V	3.5 μV/V		2.7 μV/V	-	3.7 μV/V	5.6 μV/V	9.9 μV/V	10 μV/V	10 μV/V	
30 kHz	8.5 μV/V	3.1 μV/V	4.5 μV/V	25 μV/V	2.7 μV/V	-	3.9 μV/V	7.3 μV/V	11 μV/V	12 μV/V	12 μV/V	
50 kHz	8.2 μV/V	4.3 μV/V	-	-	4 μV/V	-	6.7 μV/V	8.7 μV/V	14 μV/V	16 μV/V	-	
100 kHz	9.4 μV/V	4.6 μV/V	4.7 μV/V	32 μV/V	5.2 μV/V	-	7.3 μV/V	15 μV/V	25 μV/V	23 μV/V	-	
200 kHz	21 μV/V	7.9 μV/V	-	-	7.6 μV/V	-	13 μV/V	-	-	-	-	
300 kHz	21 μV/V	7.7 μV/V	7.5 μV/V	35 μV/V	7.6 μV/V	-	-	-	-	-	-	
500 kHz	25 μV/V	11 μV/V	-	-	11 μV/V	-	-	-	-	-	-	
1 MHz	33 μV/V	18 μV/V	17 μV/V	52 μV/V	18 μV/V	-	-	-	-	-	-	

**Electrical – DC/Low Frequency**

**Main Scope**

Parameter/Equipment		AC DC Difference - Measure									
Reference Standard, Method, and/or Equipment		Comparison to an AC DC transfer standard and a ratio transformer									
Expanded Uncertainty of Measurement (+/-)											
Range	200 mV	600 mV	1 V	2 V	6 V	20 V	60 V	200 V	600 V	1000 V	
10 Hz	31 μV/V	14 μV/V	12 μV/V	33 μV/V	25 μV/V	22 μV/V	14 μV/V	23 μV/V	-	-	
20 Hz	22 μV/V	12 μV/V	13 μV/V	4.2 μV/V	4.6 μV/V	10 μV/V	8.5 μV/V	15 μV/V	-	-	
40 Hz	13 μV/V	11 μV/V	3.2 μV/V	2.4 μV/V	3.2 μV/V	6.3 μV/V	10 μV/V	12 μV/V	12 μV/V	12 μV/V	
1 kHz	9.8 μV/V	5.4 μV/V	3 μV/V	5.8 μV/V	6.5 μV/V	6.8 μV/V	11 μV/V	11 μV/V	12 μV/V	12 μV/V	
20 kHz	9.7 μV/V	5.8 μV/V	2.8 μV/V	2.7 μV/V	2.3 μV/V	6.3 μV/V	6.2 μV/V	11 μV/V	11 μV/V	11 μV/V	
50 kHz	10 μV/V	5.8 μV/V	3 μV/V	2.8 μV/V	2.4 μV/V	6.1 μV/V	6.3 μV/V	11 μV/V	-	-	

**Electrical – DC/Low Frequency**

**Main Scope**

Parameter/Equipment		AC Voltage Flatness - Measure						
Reference Standard, Method, and/or Equipment		Comparison to a Thermal Voltage Convertor, reference attenuators						
Expanded Uncertainty of Measurement (+/-)								
Range	(0.6 to 2.2) mV	(1.9 to 7) mV	(6 to 22) mV	(19 to 70) mV	(60 to 220) mV	(190 to 700) mV	(0.6 to 2.2) V	(1.9 to 7) V
(10 to 20) Hz	77 μV/V	72 μV/V	71 μV/V	70 μV/V	70 μV/V	70 μV/V	70 μV/V	70 μV/V
(20 to 50) Hz	75 μV/V	70 μV/V	70 μV/V	70 μV/V	70 μV/V	70 μV/V	70 μV/V	70 μV/V
(50 to 100) Hz	78 μV/V	70 μV/V	70 μV/V	70 μV/V	70 μV/V	70 μV/V	70 μV/V	70 μV/V
(0.1 to 1) kHz	41 μV/V	45 μV/V	43 μV/V	41 μV/V	40 μV/V	40 μV/V	40 μV/V	40 μV/V
(1 to 20) kHz	45 μV/V	40 μV/V	40 μV/V	40 μV/V	40 μV/V	40 μV/V	40 μV/V	40 μV/V
(20 to 50) kHz	47 μV/V	40 μV/V	40 μV/V	40 μV/V	40 μV/V	40 μV/V	40 μV/V	40 μV/V
(50 to 100) kHz	45 μV/V	40 μV/V	40 μV/V	40 μV/V	40 μV/V	40 μV/V	40 μV/V	40 μV/V
(100 to 200) kHz	56 μV/V	50 μV/V	50 μV/V	50 μV/V	50 μV/V	50 μV/V	50 μV/V	50 μV/V
(200 to 300) kHz	68 μV/V	62 μV/V	61 μV/V	60 μV/V	60 μV/V	60 μV/V	60 μV/V	60 μV/V
(300 to 500) kHz	66 μV/V	65 μV/V	62 μV/V	62 μV/V	61 μV/V	60 μV/V	60 μV/V	60 μV/V
(0.5 to 1) MHz	93 μV/V	90 μV/V	85 μV/V	84 μV/V	83 μV/V	81 μV/V	80 μV/V	80 μV/V
(1 to 2) MHz	0.12 mV/V	0.11 mV/V	99 μV/V	94 μV/V	90 μV/V	85 μV/V	80 μV/V	81 μV/V
(2 to 3) MHz	0.27 mV/V	0.26 mV/V	0.24 mV/V	0.23 mV/V	0.22 mV/V	0.21 mV/V	0.21 mV/V	0.21 mV/V
(3 to 4) MHz	0.33 mV/V	0.32 mV/V	0.27 mV/V	0.25 mV/V	0.24 mV/V	0.22 mV/V	0.21 mV/V	0.21 mV/V
(4 to 8) MHz	0.48 mV/V	0.46 mV/V	0.4 mV/V	0.38 mV/V	0.36 mV/V	0.35 mV/V	0.33 mV/V	0.33 mV/V
(8 to 10) MHz	0.77 mV/V	0.74 mV/V	0.57 mV/V	0.52 mV/V	0.46 mV/V	0.4 mV/V	0.33 mV/V	0.33 mV/V
(10 to 15) MHz	0.95 mV/V	0.9 mV/V	0.68 mV/V	0.61 mV/V	0.54 mV/V	0.46 mV/V	0.36 mV/V	0.36 mV/V
(15 to 20) MHz	1 mV/V	1 mV/V	0.83 mV/V	0.78 mV/V	0.72 mV/V	0.66 mV/V	0.6 mV/V	0.6 mV/V
(20 to 26) MHz	1 mV/V	1 mV/V	0.83 mV/V	0.78 mV/V	0.72 mV/V	0.66 mV/V	0.6 mV/V	0.6 mV/V
(26 to 30) MHz	1.2 mV/V	1.1 mV/V	1 mV/V	0.97 mV/V	0.92 mV/V	0.88 mV/V	0.83 mV/V	0.83 mV/V
(30 to 35) MHz	2 mV/V	1.7 mV/V	1.7 mV/V	1.4 mV/V	1.3 mV/V	1.1 mV/V	1.1 mV/V	1.1 mV/V
(35 to 40) MHz	2.2 mV/V	1.9 mV/V	1.9 mV/V	1.5 mV/V	1.4 mV/V	1.2 mV/V	1.2 mV/V	1.2 mV/V
(45 to 50) MHz	2.4 mV/V	2.1 mV/V	2.1 mV/V	1.7 mV/V	1.6 mV/V	1.3 mV/V	1.3 mV/V	1.3 mV/V

**Electrical – DC/Low Frequency**

**Main Scope**

<b>Parameter/Equipment</b>	AC Voltage - Source and Measure				
<b>Reference Standard, Method, and/or Equipment</b>	Comparison to an AC source and a voltage divider				
<b>Expanded Uncertainty of Measurement (+/-)</b>					
<b>Range</b>	(0.6 to 2.2) mV	(1.9 to 7) mV	(6 to 22) mV	(19 to 70) mV	(60 to 220) mV
(10 to 20) Hz	15 $\mu$ V/V	5.2 $\mu$ V/V	4.2 $\mu$ V/V	3.6 $\mu$ V/V	3.4 $\mu$ V/V
(20 to 45) Hz	14 $\mu$ V/V	4 $\mu$ V/V	4.2 $\mu$ V/V	3.5 $\mu$ V/V	3.3 $\mu$ V/V
(45 to 100) Hz	13 $\mu$ V/V	5.4 $\mu$ V/V	4 $\mu$ V/V	3.4 $\mu$ V/V	3.4 $\mu$ V/V
(0.1 to 1) kHz	19 $\mu$ V/V	4.5 $\mu$ V/V	4.2 $\mu$ V/V	3.4 $\mu$ V/V	10 $\mu$ V/V
(1 to 20) kHz	22 $\mu$ V/V	11 $\mu$ V/V	11 $\mu$ V/V	10 $\mu$ V/V	5.3 $\mu$ V/V
(20 to 50) kHz	46 $\mu$ V/V	6.6 $\mu$ V/V	5.8 $\mu$ V/V	5.4 $\mu$ V/V	5.4 $\mu$ V/V
(50 to 100) kHz	45 $\mu$ V/V	6.1 $\mu$ V/V	5 $\mu$ V/V	5.4 $\mu$ V/V	5.4 $\mu$ V/V
(100 to 200) kHz	46 $\mu$ V/V	5.3 $\mu$ V/V	4.8 $\mu$ V/V	7.4 $\mu$ V/V	7.4 $\mu$ V/V
(200 to 300) kHz	35 $\mu$ V/V	10 $\mu$ V/V	9 $\mu$ V/V	7.8 $\mu$ V/V	7.8 $\mu$ V/V
(300 to 500) kHz	58 $\mu$ V/V	22 $\mu$ V/V	21 $\mu$ V/V	25 $\mu$ V/V	25 $\mu$ V/V
(0.5 to 1) MHz	328 $\mu$ V/V	114 $\mu$ V/V	114 $\mu$ V/V	49 $\mu$ V/V	49 $\mu$ V/V

**Electrical – DC/Low Frequency**

**Main Scope**

<b>Parameter/Equipment</b>	AC Voltage - Measure														
<b>Reference Standard, Method, and/or Equipment</b>	Comparison to an AC DC transfer standard														
<b>Expanded Uncertainty of Measurement (+/-)</b>															
<b>Range</b>	10 Hz	20 Hz	40 Hz	45 Hz	100 Hz	1 kHz	10 kHz	20 kHz	30 kHz	50 kHz	100 kHz	200 kHz	300 kHz	500 kHz	1 MHz
60 mV	49 $\mu$ V/V	38 $\mu$ V/V	37 $\mu$ V/V	-	-	40 $\mu$ V/V	-	37 $\mu$ V/V	-	26 $\mu$ V/V	38 $\mu$ V/V	-	81 $\mu$ V/V	81 $\mu$ V/V	81 $\mu$ V/V
200 mV	27 $\mu$ V/V	20 $\mu$ V/V	11 $\mu$ V/V	-	-	7 $\mu$ V/V	-	7 $\mu$ V/V	-	8 $\mu$ V/V	9 $\mu$ V/V	-	30 $\mu$ V/V	30 $\mu$ V/V	47 $\mu$ V/V
300 mV	15 $\mu$ V/V	13 $\mu$ V/V	12 $\mu$ V/V	12 $\mu$ V/V	13 $\mu$ V/V	6.8 $\mu$ V/V	9.5 $\mu$ V/V	9.5 $\mu$ V/V	10 $\mu$ V/V	10 $\mu$ V/V	10 $\mu$ V/V	21 $\mu$ V/V	21 $\mu$ V/V	26 $\mu$ V/V	35 $\mu$ V/V
500 mV	-	-	-	-	-	6.8 $\mu$ V/V	-	-	-	-	-	-	-	-	-
600 mV	13 $\mu$ V/V	12 $\mu$ V/V	11 $\mu$ V/V	-	-	5.8 $\mu$ V/V	-	6 $\mu$ V/V	-	5.8 $\mu$ V/V	8.6 $\mu$ V/V	-	30 $\mu$ V/V	30 $\mu$ V/V	45 $\mu$ V/V
1 V	3.1 $\mu$ V/V	2.2 $\mu$ V/V	1.6 $\mu$ V/V	1.6 $\mu$ V/V	1.6 $\mu$ V/V	1.6 $\mu$ V/V	1.3 $\mu$ V/V	1.7 $\mu$ V/V	1.4 $\mu$ V/V	1.9 $\mu$ V/V	4.1 $\mu$ V/V	5.1 $\mu$ V/V	5.1 $\mu$ V/V	9.1 $\mu$ V/V	9.1 $\mu$ V/V

**Electrical – DC/Low Frequency**

**Main Scope**

Parameter/Equipment	AC Voltage - Measure														
Reference Standard, Method, and/or Equipment	Comparison to an AC DC transfer standard														
Expanded Uncertainty of Measurement (+/-)															
Range	10 Hz	20 Hz	40 Hz	45 Hz	100 Hz	1 kHz	10 kHz	20 kHz	30 kHz	50 kHz	100 kHz	200 kHz	300 kHz	500 kHz	1 MHz
2 V	28 $\mu$ V/V	5.6 $\mu$ V/V	4.7 $\mu$ V/V	-	-	5.8 $\mu$ V/V	-	3.1 $\mu$ V/V	-	5.9 $\mu$ V/V	6.1 $\mu$ V/V	-	11 $\mu$ V/V	10 $\mu$ V/V	16 $\mu$ V/V
3 V	-	-	-	-	-	1.7 $\mu$ V/V	-	-	-	-	5.1 $\mu$ V/V	-	-	-	-
6 V	20 $\mu$ V/V	5.7 $\mu$ V/V	4.1 $\mu$ V/V	-	-	1.5 $\mu$ V/V	-	3.4 $\mu$ V/V	-	2.8 $\mu$ V/V	5.2 $\mu$ V/V	-	10 $\mu$ V/V	10 $\mu$ V/V	19 $\mu$ V/V
10 V	2.5 $\mu$ V/V	2.2 $\mu$ V/V	1.8 $\mu$ V/V	1.8 $\mu$ V/V	1.6 $\mu$ V/V	1.7 $\mu$ V/V	1.6 $\mu$ V/V	1.4 $\mu$ V/V	1.5 $\mu$ V/V	1.6 $\mu$ V/V	4.1 $\mu$ V/V	5.1 $\mu$ V/V	5.1 $\mu$ V/V	9.1 $\mu$ V/V	9.1 $\mu$ V/V
20 V	17 $\mu$ V/V	9.9 $\mu$ V/V	6.9 $\mu$ V/V	-	-	7.8 $\mu$ V/V	-	6.3 $\mu$ V/V	-	6.3 $\mu$ V/V	7.1 $\mu$ V/V	-	12 $\mu$ V/V	12 $\mu$ V/V	25 $\mu$ V/V
60 V	13 $\mu$ V/V	8 $\mu$ V/V	8.1 $\mu$ V/V	-	-	9.9 $\mu$ V/V	-	6.5 $\mu$ V/V	-	6.6 $\mu$ V/V	12 $\mu$ V/V	-	14 $\mu$ V/V	-	-
100 V	-	-	-	-	-	-	-	-	-	-	-	-	7.1 $\mu$ V/V	-	-
200 V	5.1 $\mu$ V/V	5.1 $\mu$ V/V	5.1 $\mu$ V/V	5.1 $\mu$ V/V	5.1 $\mu$ V/V	5.1 $\mu$ V/V	5.1 $\mu$ V/V	5.1 $\mu$ V/V	5.1 $\mu$ V/V	5.1 $\mu$ V/V	8.1 $\mu$ V/V	10 $\mu$ V/V	-	-	-
300 V	22 $\mu$ V/V	15 $\mu$ V/V	12 $\mu$ V/V	-	-	12 $\mu$ V/V	-	11 $\mu$ V/V	-	11 $\mu$ V/V	11 $\mu$ V/V	-	-	-	-
500 V	-	-	6.1 $\mu$ V/V	6.1 $\mu$ V/V	6.1 $\mu$ V/V	6.1 $\mu$ V/V	6.1 $\mu$ V/V	6.1 $\mu$ V/V	6.1 $\mu$ V/V	6.1 $\mu$ V/V	12 $\mu$ V/V	-	-	-	-
600 V	-	-	9.1 $\mu$ V/V	9.1 $\mu$ V/V	9.1 $\mu$ V/V	9.1 $\mu$ V/V	9.1 $\mu$ V/V	9.1 $\mu$ V/V	9.1 $\mu$ V/V	11 $\mu$ V/V	18 $\mu$ V/V	-	-	-	-
700 V	-	-	12 $\mu$ V/V	-	-	12 $\mu$ V/V	-	11 $\mu$ V/V	-	11 $\mu$ V/V	35 $\mu$ V/V	-	-	-	-
1 000 V	-	-	6.1 $\mu$ V/V	6.1 $\mu$ V/V	6.1 $\mu$ V/V	6.1 $\mu$ V/V	6.1 $\mu$ V/V	6.1 $\mu$ V/V	6.1 $\mu$ V/V	6.1 $\mu$ V/V	12 $\mu$ V/V	-	-	-	-

**Electrical – DC/Low Frequency**

**Main Scope**

Parameter/Equipment	AC Voltage - Source							
Reference Standard, Method, and/or Equipment	Comparison to a characterized AC voltage source							
Expanded Uncertainty of Measurement (+/-)								
Range	10 mV	100 mV	1 V	3 V	10 V	100 V	700 V	1000 V
10 Hz	0.69 $\mu$ V	1.7 $\mu$ V	-	-	76 $\mu$ V	-	-	-
20 Hz	0.51 $\mu$ V	1.8 $\mu$ V	-	-	45 $\mu$ V	-	-	-
40 Hz	-	-	-	-	35 $\mu$ V	-	-	-
200 Hz	-	-	-	-	24 $\mu$ V	-	-	-

**Electrical – DC/Low Frequency**

**Main Scope**

Parameter/Equipment	AC Voltage - Source							
Reference Standard, Method, and/or Equipment	Comparison to a characterized AC voltage source							
Expanded Uncertainty of Measurement (+/-)								
Range	10 mV	100 mV	1 V	3 V	10 V	100 V	700 V	1000 V
500 Hz	-	-	-	-	25 µV	-	-	-
1 kHz	70 nV	0.36 µV	2.6 µV	-	26 µV	0.42 mV	6.5 mV	16 mV
10 kHz	-	-	-	-	26 µV	-	7.0 mV	11 mV
20 kHz	76 nV	0.31 µV	2.8 µV	-	25 µV	0.35 mV	-	22 mV
50 kHz	-	-	3.7 µV	-	36 µV	0.67 mV	-	-
100 kHz	62 nV	0.34 µV	4.6 µV	13 µV	44 µV	0.80 mV	-	-
300 kHz	0.17 µV	0.7 µV	8 µV	-	73 µV	-	-	-
500 kHz	-	-	11 µV	-	0.11 mV	-	-	-
1 MHz	1.15 µV	2.7 µV	20 µV	-	0.19 mV	-	-	-
2 MHz	-	-	-	2.1 mV	-	-	-	-
4 MHz	10 µV	0.1 mV	1 mV	3.2 mV	-	-	-	-
8 MHz	-	0.16 mV	1.6 mV	4.8 mV	-	-	-	-
10 MHz	-	0.18 mV	1.8 mV	5.5 mV	-	-	-	-

**Electrical – DC/Low Frequency**

**Main Scope**

Parameter/Equipment	AC Voltage - Source								
Reference Standard, Method, and/or Equipment	Comparison to an AC voltage source								
Expanded Uncertainty of Measurement (+/-)									
Range	(>0 to 2.2) mV	(2.2 to 22) mV	(22 to 220) mV	(0.22 to 2.2) V	(2.2 to 22) V	(22 to 220) V	(220 to 250) V	(220 to 100) V	(220 to 750) V
(10 to 15) Hz	230 µV/V + 3.9 µV	230 µV/V + 3.9 µV	230 µV/V + 12 µV	230 µV/V + 39 µV	230 µV/V + 390 µV	230 µV/V + 3.9 mV	-	-	-
(15 to 20) Hz	230 µV/V + 3.9 µV	230 µV/V + 3.9 µV	230 µV/V + 12 µV	230 µV/V + 39 µV	230 µV/V + 390 µV	230 µV/V + 3.9 mV	280 µV/V + 16 mV	-	-
(20 to 40) Hz	89 µV/V + 3.9 µV	89 µV/V + 3.9 µV	89 µV/V + 6.2 µV	85 µV/V + 16 µV	85 µV/V + 160 µV	85 µV/V + 1.6 mV	280 µV/V + 16 mV	-	-
(40 to 50) Hz	77 µV/V + 3.9 µV	77 µV/V + 3.9 µV	54 µV/V + 6.2 µV	37 µV/V + 7.8 µV	37 µV/V + 54 µV	50 µV/V + 0.54 mV	-	70 µV/V + 3.1 mV	-
50 Hz to 1 kHz	77 µV/V + 3.9 µV	77 µV/V + 3.9 µV	54 µV/V + 6.2 µV	37 µV/V + 7.8 µV	37 µV/V + 54 µV	50 µV/V + 0.54 mV	-	66 µV/V + 3.1 mV	-
(1 to 20) kHz	77 µV/V + 3.9 µV	77 µV/V + 3.9 µV	54 µV/V + 6.2 µV	37 µV/V + 7.8 µV	37 µV/V + 54 µV	50 µV/V + 0.54 mV	-	130 µV/V + 4.7 mV	-
(20 to 30) kHz	190 µV/V + 3.9 µV	190 µV/V + 3.9 µV	120 µV/V + 6.2 µV	62 µV/V + 9.3 µV	62 µV/V + 93 µV	78 µV/V + 0.93 mV	-	470 µV/V + 8.5 mV	-



ANSI National Accreditation Board

Electrical – DC/Low Frequency

Main Scope

Parameter/Equipment		AC Voltage - Source							
Reference Standard, Method, and/or Equipment		Comparison to an AC voltage source							
Expanded Uncertainty of Measurement (+/-)									
Range	(>0 to 2.2) mV	(2.2 to 22) mV	(22 to 220) mV	(0.22 to 2.2) V	(2.2 to 22) V	(22 to 220) V	(220 to 250) V	(220 to 100) V	(220 to 750) V
(30 to 50) kHz	190 $\mu$ V/V + 3.9 $\mu$ V	190 $\mu$ V/V + 3.9 $\mu$ V	120 $\mu$ V/V + 6.2 $\mu$ V	62 $\mu$ V/V + 9.3 $\mu$ V	62 $\mu$ V/V + 93 $\mu$ V	78 $\mu$ V/V + 0.93 mV	-	-	470 $\mu$ V/V + 8.5 mV
(50 to 100) kHz	460 $\mu$ V/V + 4.7 $\mu$ V	470 $\mu$ V/V + 4.7 $\mu$ V	310 $\mu$ V/V + 16 $\mu$ V	78 $\mu$ V/V + 31 $\mu$ V	78 $\mu$ V/V + 190 $\mu$ V	140 $\mu$ V/V + 2.3 mV	-	-	1.8 mV/V + 35 mV
Range	(>0 to 2.2) mV	(2.2 to 22) mV	(22 to 220) mV	(0.22 to 2.2) V	(2.2 to 22) V	(22 to 2.2e7/freq) V	(220 to 250) V	(220 to 100) V	(220 to 250) V
(100 to 300) kHz	1 mV/V + 9.3 $\mu$ V	1 mV/V + 9.3 $\mu$ V	620 $\mu$ V/V + 19 $\mu$ V	310 $\mu$ V/V + 78 $\mu$ V	230 $\mu$ V/V + 620 $\mu$ V	850 $\mu$ V/V + 16 mV	-	-	-
(300 to 500) kHz	1.3 mV/V + 19 $\mu$ V	1.3 mV/V + 19 $\mu$ V	1.3 mV/V + 23 $\mu$ V	930 $\mu$ V/V + 190 $\mu$ V	930 $\mu$ V/V + 1.9 mV	4.2 mV/V + 39 mV	-	-	-
500 kHz to 1 MHz	2.6 mV/V + 19 $\mu$ V	2.6 mV/V + 19 $\mu$ V	2.6 mV/V + 47 $\mu$ V	1.6 mV/V + 310 $\mu$ V	1.4 mV/V + 3.1 mV	7.8 mV/V + 78 mV	-	-	-

Electrical – DC/Low Frequency

Main Scope

Parameter/Equipment		AC Voltage - Measure				
Reference Standard, Method, and/or Equipment		Comparison to a Keysight 3458A multimeter				
Expanded Uncertainty of Measurement (+/-)						
Range	(>0 to 10 mV)	(10 to 120) mV	(0.12 to 1.2) V	(1.2 to 12) V	(12 to 120) V	(120 to 700) V
(1 to 40) Hz	0.35 mV/V + 3.4 $\mu$ V	83 $\mu$ V/V + 4.6 $\mu$ V	83 $\mu$ V/V + 46 $\mu$ V	83 $\mu$ V/V + 0.46 mV	0.23 mV/V + 4.6 mV	0.46 mV/V + 46 mV
40 Hz to 1 kHz	0.23 mV/V + 1.3 $\mu$ V	83 $\mu$ V/V + 2.3 $\mu$ V	83 $\mu$ V/V + 23 $\mu$ V	83 $\mu$ V/V + 0.23 mV	0.23 mV/V + 2.3 mV	0.46 mV/V + 23 mV
(1 to 20) kHz	0.34 mV/V + 1.3 $\mu$ V	0.16 mV/V + 2.3 $\mu$ V	0.16 mV/V + 23 $\mu$ V	0.16 mV/V + 0.23 mV	0.23 mV/V + 2.3 mV	0.7 mV/V + 23 mV
(20 to 50) kHz	1.1 mV/V + 1.3 $\mu$ V	0.34 mV/V + 2.3 $\mu$ V	0.34 mV/V + 23 $\mu$ V	0.34 mV/V + 0.23 mV	0.4 mV/V + 2.3 mV	1.4 mV/V + 23 mV
(50 to 100) kHz	5.7 mV/V + 1.2 $\mu$ V	0.92 mV/V + 2.3 $\mu$ V	0.92 mV/V + 23 $\mu$ V	0.92 mV/V + 0.23 mV	1.4 mV/V + 2.3 mV	3.5 mV/V + 23 mV
(100 to 300) kHz	46 mV/V + 2.3 $\mu$ V	3.4 mV/V + 12 $\mu$ V	3.4 mV/V + 0.11 mV	3.4 mV/V + 1.2 mV	4.6 mV/V + 11 mV	-
300 kHz to 1 MHz	14 mV/V + 5.8 $\mu$ V	11 mV/V + 12 $\mu$ V	11 mV/V + 0.12 mV	11 mV/V + 1.2 mV	17 mV/V + 11 mV	-
(1 to 2) MHz	81 mV/V + 8.1 $\mu$ V	17 mV/V + 12 $\mu$ V	17 mV/V + 0.12 mV	17 mV/V + 1.2 mV	-	-

**Electrical – DC/Low Frequency**

**Main Scope**

<b>Parameter/Equipment</b>	AC Voltage - Measure					
<b>Reference Standard, Method, and/or Equipment</b>	Comparison to a Keysight 3458A multimeter					
<b>Expanded Uncertainty of Measurement (+/-)</b>						
<b>Range</b>	(>0 to 10 mV)	(10 to 120) mV	(0.12 to 1.2) V	(1.2 to 12) V	(12 to 120) V	(120 to 700) V
(2 to 4) MHz	82 mV/V + 8.1 μV	46 mV/V + 81 μV	46 mV/V + 0.81 mV	46 mV/V + 8.1 mV	-	-
(4 to 8) MHz	230 mV/V + 9.2 μV	46 mV/V + 92 μV	46 mV/V + 0.92 mV	46 mV/V + 9.2 mV	-	-
(8 to 10) MHz	-	170 mV/V + 120 μV	170 mV/V + 1.2 mV	170 mV/V + 12 mV	-	-

**Electrical – DC/Low Frequency**

**Main Scope**

<b>Parameter/Equipment</b>	AC Current - Source								
<b>Reference Standard, Method, and/or Equipment</b>	Comparison to an AC source								
<b>Expanded Uncertainty of Measurement (+/-)</b>									
<b>Range</b>	(10 to 20) Hz	(20 to 30) Hz	(30 to 40) Hz	(40 to 45) Hz	(45 to 100) Hz	(0.1 to 1) kHz	(1 to 5) kHz	(5 to 10) kHz	(10 to 30) kHz
(>0 to 220) μA	230 μA/A + 16 nA	160 μA/A + 9.3 nA	160 μA/A + 9.3 nA	93 μA/A + 7.8 nA	93 μA/A + 7.8 nA	93 μA/A + 7.8 nA	270 μA/A + 12 nA	1 mA/A + 62 nA	13 mA/A + 0.33 μA
(220 to 330) μA	230 μA/A + 39 nA	160 μA/A + 31 nA	160 μA/A + 31 nA	93 μA/A + 31 nA	93 μA/A + 31 nA	93 μA/A + 31 nA	190 μA/A + 100 nA	1 mA/A + 620 nA	13 mA/A + 0.33 μA
(0.33 to 2.2) mA	230 μA/A + 39 nA	160 μA/A + 31 nA	160 μA/A + 31 nA	93 μA/A + 31 nA	93 μA/A + 31 nA	93 μA/A + 31 nA	190 μA/A + 100 nA	1 mA/A + 620 nA	8.2 mA/A + 0.49 μA
(2.2 to 3.3) mA	230 μA/A + 390 nA	160 μA/A + 310 nA	160 μA/A + 310 nA	93 μA/A + 310 nA	93 μA/A + 310 nA	93 μA/A + 310 nA	190 μA/A + 540 nA	1 mA/A + 4.7 μA	8.2 mA/A + 0.49 μA
(3.3 to 22) mA	230 μA/A + 390 nA	160 μA/A + 310 nA	160 μA/A + 310 nA	93 μA/A + 310 nA	93 μA/A + 310 nA	93 μA/A + 310 nA	190 μA/A + 540 nA	1 mA/A + 4.7 μA	3.3 mA/A + 3.3 μA
(22 to 33) mA	230 μA/A + 3.9 μA	160 μA/A + 3.1 μA	160 μA/A + 3.1 μA	93 μA/A + 2.3 μA	93 μA/A + 2.3 μA	93 μA/A + 2.3 μA	190 μA/A + 3.1 μA	1 mA/A + 9.3 μA	3.3 mA/A + 3.3 μA
(33 to 220) mA	230 μA/A + 3.9 μA	160 μA/A + 3.1 μA	160 μA/A + 3.1 μA	93 μA/A + 2.3 μA	93 μA/A + 2.3 μA	93 μA/A + 2.3 μA	190 μA/A + 3.1 μA	1 mA/A + 9.3 μA	3.3 mA/A + 0.16 mA
(220 to 330) mA	1.5 mA/A + 16 μA	230 μA/A + 31 μA	230 μA/A + 31 μA	230 μA/A + 31 μA	230 μA/A + 31 μA	230 μA/A + 31 μA	390 μA/A + 78 μA	6.2 mA/A + 160 μA	3.3 mA/A + 0.16 mA
(0.33 to 2.2) A	1.5 mA/A + 82 μA	230 μA/A + 31 μA	230 μA/A + 31 μA	230 μA/A + 31 μA	230 μA/A + 31 μA	230 μA/A + 31 μA	390 μA/A + 78 μA	6.2 mA/A + 160 μA	-
(2.2 to 3) A	1.5 mA/A + 82 μA	1.5 mA/A + 82 μA	1.5 mA/A + 82 μA	360 μA/A + 130 μA	360 μA/A + 130 μA	360 μA/A + 130 μA	740 μA/A + 290 μA	2.8 mA/A + 580 μA	-
(3 to 11) A	-	-	-	360 μA/A + 130 μA	360 μA/A + 130 μA	360 μA/A + 130 μA	740 μA/A + 290 μA	2.8 mA/A + 580 μA	-
(11 to 20.5) A	-	-	-	-	0.98 mA/A + 4.1 mA	1.2 mA/A + 4.1 mA	25 mA/A + 4.1 mA	-	-

**Electrical – DC/Low Frequency**

**Main Scope**

Parameter/Equipment	AC Current - Measure										
Reference Standard, Method, and/or Equipment	Comparison to an AC measurement standard, source and reference current shunts										
Expanded Uncertainty of Measurement (+/-)											
Range	10 Hz	20 Hz	40 Hz	50 Hz	60 Hz	400 Hz	500 Hz	1 kHz	3 kHz	5 kHz	10 kHz
10 $\mu$ A	0.5 nA	0.71 nA	-	0.48 nA	-	-	-	0.44 nA	-	-	-
100 $\mu$ A	4.6 nA	4.5 nA	-	4.5 nA	-	-	-	4.5 nA	-	4.6 nA	4.6 nA
1 mA	39 nA	39 nA	-	39 nA	-	-	-	39 nA	-	40 nA	38 nA
10 mA	0.25 $\mu$ A	0.25 $\mu$ A	-	0.24 $\mu$ A	-	-	-	0.24 $\mu$ A	-	0.25 $\mu$ A	0.25 $\mu$ A
100 mA	4.7 $\mu$ A	4.7 $\mu$ A	-	4.7 $\mu$ A	-	-	-	4.7 $\mu$ A	-	4.7 $\mu$ A	4.3 $\mu$ A
1 A	36 $\mu$ A	36 $\mu$ A	-	36 $\mu$ A	-	-	-	36 $\mu$ A	-	37 $\mu$ A	41 $\mu$ A
2.5 A	-	-	-	-	0.6 mA	-	1.1 mA	-	-	-	-
5 A	-	-	-	-	1.1 mA	-	2.4 mA	-	-	-	-
10 A	-	-	0.55 mA	-	4.9 mA	0.55 mA	4.9 mA	0.48 mA	0.71 mA	0.61 mA	0.49 mA
20 A	-	-	-	-	9.5 mA	-	9.5 mA	-	-	-	-
40 A	-	-	-	-	19 mA	-	19 mA	-	-	-	-

**Electrical – DC/Low Frequency**

**Main Scope**

Parameter/Equipment	AC Current - Measure										
Reference Standard, Method, and/or Equipment	Comparison to an AC measurement standard, source and reference current shunts										
Expanded Uncertainty of Measurement (+/-)											
Range	10 Hz	20 Hz	40 Hz	45 Hz	65 Hz	500 Hz	1 kHz	5 kHz	10 kHz	30 kHz	
20 $\mu$ A	-	-	-	-	-	-	2.7 nA	-	2.7 nA	-	
33 $\mu$ A	-	-	-	-	-	-	4.9 nA	-	10 nA	8.3 nA	
190 $\mu$ A	-	-	-	9.8 nA	-	-	9.7 nA	9.7 nA	9.7 nA	14 nA	
200 $\mu$ A	34 nA	15 nA	7.8 nA	-	-	-	7.7 nA	7.6 nA	7.8 nA	-	
329 $\mu$ A	56 nA	-	-	15 nA	-	-	15 nA	15 nA	15 nA	19 nA	
330 $\mu$ A	-	-	-	-	-	-	20 nA	19 nA	-	21 nA	
1.9 mA	-	-	-	-	-	-	85 nA	85 nA	85 nA	130 nA	
2 mA	350 nA	150 nA	87 nA	-	-	-	87 nA	88 nA	88 nA	-	
3.29 mA	560 nA	-	-	130 nA	-	-	130 nA	130 nA	130 nA	170 nA	
3.3 mA	-	-	-	-	-	-	180 nA	140 nA	140 nA	240 nA	
19 mA	-	-	-	-	-	-	580 nA	-	590 nA	830 nA	
20 mA	3.2 $\mu$ A	1.1 $\mu$ A	0.6 $\mu$ A	-	-	-	0.6 $\mu$ A	0.6 $\mu$ A	0.6 $\mu$ A	-	
32.9 mA	5.6 $\mu$ A	-	-	1.3 $\mu$ A	-	-	1.3 $\mu$ A	1.3 $\mu$ A	1.3 $\mu$ A	1.7 $\mu$ A	
33 mA	-	-	-	-	-	-	1.5 $\mu$ A	1.7 $\mu$ A	-	2 $\mu$ A	

**Electrical – DC/Low Frequency**

**Main Scope**

Parameter/Equipment	AC Current - Measure									
Reference Standard, Method, and/or Equipment	Comparison to an AC measurement standard, source and reference current shunts									
Expanded Uncertainty of Measurement (+/-)										
Range	10 Hz	20 Hz	40 Hz	45 Hz	65 Hz	500 Hz	1 kHz	5 kHz	10 kHz	30 kHz
190 mA	-	-	-	-	-	-	6 µA	6.1 µA	-	8.6 µA
200 mA	32 µA	11 µA	6.3 µA	-	-	-	6.3 µA	6.4 µA	6.3 µA	-
329 mA	56 µA	-	-	16 µA	-	-	16 µA	16 µA	16 µA	20 µA
330 mA	-	-	-	-	-	-	18 µA	17 µA	46 µA	-
1.09 A	170 µA	-	-	36 µA	-	-	35 µA	35 µA	140 µA	-
2 A	-	0.15 mA	-	-	-	-	0.1 mA	0.1 mA	0.13 mA	-
2.19 A	-	-	-	0.11 mA	-	-	0.11 mA	0.11 mA	-	-
2.2 A	-	-	-	-	-	0.11 mA	0.11 mA	-	-	-
2.99 A	0.51 mA	-	-	0.14 mA	-	-	0.14 mA	0.14 mA	0.14 mA	-
3 A	-	-	0.14 mA	-	-	-	0.14 mA	0.14 mA	0.14 mA	-
3.3 A	-	-	-	-	-	0.23 mA	0.23 mA	0.17 mA	-	-
10 A	-	-	0.84 mA	-	-	-	0.86 mA	0.88 mA	0.89 mA	-
10.9 A	-	-	-	0.89 mA	0.88 mA	0.88 mA	0.89 mA	0.93 mA	-	-
11 A	-	-	-	0.89 mA	0.88 mA	0.88 mA	0.89 mA	0.93 mA	-	-
20 A	-	-	-	1.4 mA	0.88 mA	0.92 mA	0.91 mA	1.1 mA	-	-

**Electrical – DC/Low Frequency**

**Main Scope**

Parameter/Equipment	AC Current - Measure			
Reference Standard, Method, and/or Equipment	Comparison to a Keysight 3458A multimeter			
Expanded Uncertainty of Measurement (+/-)				
Range	(10 to 20) Hz	(20 to 45) Hz	(45 to 100) Hz	(0.1 to 5) kHz
(>0 to 120) µA	4.6 mA/A + 34 nA	1.7 mA/A + 34 nA	0.69 mA/A + 34 nA	0.69 mA/A + 34 nA
(0.1 to 1.2) mA	4.6 mA/A + 0.23 µA	1.7 mA/A + 0.23 µA	0.69 mA/A + 0.23 µA	0.35 mA/A + 0.23 µA
(1 to 12) mA	4.6 mA/A + 2.3 µA	1.7 mA/A + 2.3 µA	0.69 mA/A + 2.3 µA	0.35 mA/A + 2.3 µA
(10 to 120) mA	4.6 mA/A + 23 µA	1.7 mA/A + 23 µA	0.69 mA/A + 23 µA	0.35 mA/A + 23 µA
(0.12 to 1.05) A	4.6 mA/A + 0.23 mA	1.8 mA/A + 0.23 mA	0.93 mA/A + 0.23 mA	1.1 mA/A + 0.23 mA

**Electrical – DC/Low Frequency**

**Main Scope**

Parameter/Equipment	AC Current - Measure							
Reference Standard, Method, and/or Equipment	Comparison to an AC source and a current coil							
Expanded Uncertainty of Measurement (+/-)								
(% indicates % of reading where not specified)								
Range	(10 to 20) Hz	(20 to 45) Hz	(45 to 65) Hz	(45 to 100) Hz	45 Hz to 1 kHz	(65 to 400) Hz	(0.1 to 1) kHz	(1 to 5) kHz
(0.1 to 1) mA	0.13% + 0.43 μA	0.078% + 0.47 μA	-	-	0.058% + 0.5 μA	-	-	0.13% + 0.53 μA
(1 to 3) mA	0.15% + 0.25 μA	0.095% + 0.35 μA	-	-	0.075% + 0.35 μA	-	-	0.15% + 0.35 μA
(3 to 10) mA	0.11% + 5 μA	0.063% + 4.4 μA	-	-	0.02% + 5.3 μA	-	-	0.05% + 5 μA
(10 to 30) mA	0.14% + 3 μA	0.063% + 4.4 μA	-	-	0.02% + 5.3 μA	-	-	0.050% + 5 μA
(30 to 300) mA	0.12% + 48 μA	0.063% + 44 μA	-	-	0.02% + 54 μA	-	-	0.077% + 58 μA
(0.3 to 1) A	0.15% + 86 μA	0.12% + 0.40 mA	-	-	0.02% + 0.52 mA	-	-	0.46% + 1 mA
(1 to 2.5) A	0.67% - 0.5 mA	0.46% - 0.5 mA	-	0.1%	-	-	0.14%	0.56% + 0.75 mA
(2.5 to 3) A	-	-	-	0.1%	-	-	0.14%	2.3% + 5 mA
(3 to 10) A	-	-	-	0.034% + 5.1 mA	-	-	0.058% + 5.2 mA	2.3% + 5 mA
(10 to 20) A	-	-	-	0.15% - 6.8 mA	-	-	0.18% - 7 mA	2.3% + 5 mA
(20 to 30)A	-	-	0.24% + 23 mA	-	-	0.58% + 34 mA	-	-
(30 to 150) A	-	-	0.21% + 44 mA	-	-	0.63% + 25 mA	-	-
(150 to 300) A	-	-	0.23% + 94 mA	-	-	0.64% + 71 mA	-	-
(300 to 1 020) A	-	-	0.25% + 0.19 A	-	-	0.64% + 60 mA	-	-

**Electrical – DC/Low Frequency**

**Main Scope**

Parameter/Equipment	AC Resistance - Source and Measure							
Reference Standard, Method, and/or Equipment	Comparison to reference resistors, shunts and an AC source							
Expanded Uncertainty of Measurement (+/-)								
Range	1 mΩ	4 mΩ	10 mΩ	100 mΩ	1 Ω	10 Ω	100 Ω	1 kΩ
10 Hz	-	-	-	46 μΩ/Ω	29 μΩ/Ω	30 μΩ/Ω	53 μΩ/Ω	80 μΩ/Ω
20 Hz	-	-	-	30 μΩ/Ω	30 μΩ/Ω	26 μΩ/Ω	43 μΩ/Ω	54 μΩ/Ω

**Electrical – DC/Low Frequency**

**Main Scope**

<b>Parameter/Equipment</b>	AC Resistance - Source and Measure							
<b>Reference Standard, Method, and/or Equipment</b>	Comparison to reference resistors, shunts and an AC source							
<b>Expanded Uncertainty of Measurement (+/-)</b>								
<b>Range</b>	1 mΩ	4 mΩ	10 mΩ	100 mΩ	1 Ω	10 Ω	100 Ω	1 kΩ
30 Hz	-	-	-	34 μΩ/Ω	29 μΩ/Ω	26 μΩ/Ω	38 μΩ/Ω	51 μΩ/Ω
40 Hz	287 μΩ/Ω	126 μΩ/Ω	135 μΩ/Ω	-	-	-	-	-
45 Hz	-	-	-	58 μΩ/Ω	-	-	-	-
50 Hz	-	-	-	33 μΩ/Ω	27 μΩ/Ω	28 μΩ/Ω	38 μΩ/Ω	51 μΩ/Ω
60 Hz	-	-	82 μΩ/Ω	55 μΩ/Ω	-	-	-	-
100 Hz	-	-	-	34 μΩ/Ω	28 μΩ/Ω	26 μΩ/Ω	37 μΩ/Ω	50 μΩ/Ω
300 Hz	-	-	-	30 μΩ/Ω	26 μΩ/Ω	28 μΩ/Ω	37 μΩ/Ω	51 μΩ/Ω
400 Hz	285 μΩ/Ω	116 μΩ/Ω	118 μΩ/Ω	-	-	-	-	-
500 Hz	-	-	82 μΩ/Ω	-	-	-	-	-
1 kHz	288 μΩ/Ω	110 μΩ/Ω	98 μΩ/Ω	29 μΩ/Ω	26 μΩ/Ω	28 μΩ/Ω	35 μΩ/Ω	46 μΩ/Ω
3 kHz	282 μΩ/Ω	114 μΩ/Ω	89 μΩ/Ω	30 μΩ/Ω	28 μΩ/Ω	26 μΩ/Ω	25 μΩ/Ω	47 μΩ/Ω
5 kHz	287 μΩ/Ω	103 μΩ/Ω	85 μΩ/Ω	29 μΩ/Ω	29 μΩ/Ω	27 μΩ/Ω	37 μΩ/Ω	50 μΩ/Ω
10 kHz	284 μΩ/Ω	101 μΩ/Ω	87 μΩ/Ω	33 μΩ/Ω	29 μΩ/Ω	28 μΩ/Ω	37 μΩ/Ω	49 μΩ/Ω

**Electrical – DC/Low Frequency**

**Main Scope**

<b>Parameter/Equipment</b>	AC Resistance - Source and Measure				
<b>Reference Standard, Method, and/or Equipment</b>	Comparison to reference resistors and an LCR meter				
<b>Expanded Uncertainty of Measurement (+/-)</b>					
(% indicates % of reading where not specified)					
<b>Range</b>	10 Ω	100 Ω	1 kΩ	10 kΩ	100 kΩ
100 kHz	-	-	0.022%	0.02%	0.026%
1 MHz	0.028%	0.023%	0.019%	0.025%	0.03%
2 MHz	0.042%	0.031%	0.028%	-	-
3 MHz	0.054%	0.05%	0.03%	-	-
4 MHz	0.062%	0.035%	0.031%	-	-
5 MHz	0.091%	0.048%	0.041%	-	-
10 MHz	0.32%	0.16%	0.14%	-	-
13 MHz	0.51%	0.25%	0.23%	-	-

**Electrical – DC/Low Frequency**

**Main Scope**

Parameter/Equipment		AC Resistance – Source							
Reference Standard, Method, and/or Equipment		Comparison to reference resistors							
<b>Expanded Uncertainty of Measurement (+/-)</b> (% indicates % of reading where not specified)									
Range	1 mΩ	10 mΩ	100 mΩ	1 Ω	10 Ω	100 Ω	1 kΩ	10 kΩ	100 kΩ
20 Hz	-	-	-	-	0.036%	0.0032%	0.0038%	0.023%	0.09%
100 Hz	-	-	0.03%	-	0.036%	0.044%	0.049%	0.023%	0.09%
120 Hz	-	-	-	0.014%	0.094%	0.043%	0.033%	0.023%	0.09%
125 Hz	-	-	-	-	0.094%	0.0027%	0.0037%	0.023%	0.09%
1 kHz	0.085%	0.028%	0.029%	0.0061%	0.0031%	0.003%	0.0029%	0.0064%	0.09%
12.5 kHz	-	-	-	-	0.094%	0.0029%	0.003%	0.023%	0.09%
48 kHz	-	-	-	-	0.094%	0.0033%	0.0034%	0.023%	0.09%
96 kHz	-	-	-	-	0.094%	0.0045%	0.0042%	0.023%	0.09%
100 kHz	-	-	-	-	0.094%	0.043%	0.03%	0.02%	0.0049%
1 MHz	-	-	-	-	0.096%	0.0039%	0.0042%	0.03%	0.005%
2 MHz	-	-	-	-	0.094%	0.04%	0.03%	-	-
3 MHz	-	-	-	-	0.10%	0.05%	0.03%	-	-
4 MHz	-	-	-	-	0.10%	0.05%	0.04%	-	-
5 MHz	-	-	-	-	0.12%	0.05%	0.05%	-	-
10 MHz	-	-	-	-	0.40%	0.20%	0.20%	-	-
13 MHz	-	-	-	-	0.60%	0.30%	0.30%	-	-

**Electrical – DC/Low Frequency**

**Main Scope**

Parameter/Equipment		Capacitance - Source						
Reference Standard, Method, and/or Equipment		Comparison to reference capacitors						
<b>Expanded Uncertainty of Measurement (+/-)</b> (% indicates % of reading where not specified)								
Range	1 pF	10 pF	100 pF	1000 pF	0.01 μF	0.1 μF	1 μF	10 μF
20 Hz	7.7%	5.8%	0.85%	0.083%	-	-	-	0.015%
100 Hz	5.2%	0.53%	0.046%	0.075%	0.013%	0.0097%	0.013%	0.012%
120 Hz	5.2%	0.53%	0.046%	0.075%	0.013%	0.0097%	0.013%	0.011%
125 Hz	5.2%	0.53%	0.014%	0.015%	-	-	-	-
1 kHz	0.024%	0.015%	0.012%	0.01%	0.01%	0.0097%	0.01%	0.011%
10 kHz	0.26%	0.023%	0.014%	0.018%	0.013%	0.011%	0.013%	0.019%

**Electrical – DC/Low Frequency**

**Main Scope**

Parameter/Equipment		Capacitance - Source						
Reference Standard, Method, and/or Equipment		Comparison to reference capacitors						
Expanded Uncertainty of Measurement (+/-) (% indicates % of reading where not specified)								
Range	1 pF	10 pF	100 pF	1000 pF	0.01 μF	0.1 μF	1 μF	10 μF
12.5 kHz	0.26%	0.017%	0.01%	0.011%	-	-	-	-
48 kHz	0.26%	0.016%	0.01%	0.011%	-	-	-	-
96 kHz	0.26%	0.016%	0.01%	0.011%	-	-	-	-
100 kHz	0.26%	0.016%	0.013%	0.018%	0.013%	0.0097%	0.015%	0.071%
300 kHz	0.26%	0.016%	0.01%	0.013%	-	-	-	-
500 kHz	0.26%	0.016%	0.01%	0.016%	-	-	-	-
1 MHz	0.019%	0.015%	0.01%	0.012%	-	-	-	-
2 MHz	0.031%	0.015%	0.01%	0.018%	-	-	-	-
3 MHz	0.049%	0.015%	0.015%	0.031%	-	-	-	-
4 MHz	0.068%	0.015%	0.016%	0.046%	-	-	-	-
5 MHz	0.090%	0.016%	0.019%	0.064%	-	-	-	-
10 MHz	0.25%	0.020%	0.036%	0.19%	-	-	-	-
13 MHz	0.37%	0.022%	0.051%	0.28%	-	-	-	-

**Electrical – DC/Low Frequency**

**Main Scope**

Parameter/Equipment		Capacitance - Source and Measure						
Reference Standard, Method, and/or Equipment		Comparison to reference capacitances, capacitance bridge, LCR meter and a Keysight network analyzer						
Expanded Uncertainty of Measurement (+/-) (% indicates % of reading where not specified)								
Range	1 pF	10 pF	100 pF	1000 pF	0.01 μF	0.1 μF	1 μF	10 μF
120 Hz	-	-	-	-	0.004%	0.004%	0.005%	0.005%
1 kHz	0.004 4%	0.003 9%	0.003 8%	0.004 1%	0.004%	0.004%	0.004%	0.005%
10 kHz	-	-	-	-	0.004%	0.004%	0.004%	0.016%
100 kHz	-	-	-	-	0.004%	0.004%	0.004%	0.07%
1 MHz	0.009%	0.003 9%	0.004%	0.0064%	-	-	-	-
2 MHz	0.023%	0.004%	0.004 8%	0.015%	-	-	-	-
3 MHz	0.041%	0.004 3%	0.006 6%	0.028%	-	-	-	-
4 MHz	0.063%	0.004 7%	0.009 1%	0.044%	-	-	-	-
5 MHz	0.088%	0.005 4%	0.013%	0.062%	-	-	-	-

**Electrical – DC/Low Frequency**

**Main Scope**

<b>Parameter/Equipment</b>	Capacitance - Source and Measure							
<b>Reference Standard, Method, and/or Equipment</b>	Comparison to reference capacitances, capacitance bridge, LCR meter and a Keysight network analyzer							
<b>Expanded Uncertainty of Measurement (+/-)</b> (% indicates % of reading where not specified)								
<b>Range</b>	1 pF	10 pF	100 pF	1000 pF	0.01 μF	0.1 μF	1 μF	10 μF
10 MHz	0.37%	0.012%	0.033%	0.19%	-	-	-	-
13 MHz	0.25%	0.016%	0.049%	0.28%	-	-	-	-

**Electrical – DC/Low Frequency**

**Main Scope**

<b>Parameter/Equipment</b>	Dissipation - Source							
<b>Reference Standard, Method, and/or Equipment</b>	Comparison to reference capacitors							
<b>Expanded Uncertainty of Measurement (+/-)</b>								
<b>Range</b>	1 pF	10 pF	100 pF	1 000 pF	0.01 μF	0.1 μF	1 μF	10 μF
20 Hz	-	-	0.003	0.000 31	-	-	-	0.000 073
100 Hz	0.025	0.003 9	0.000 43	0.000 46	0.000 062	-	-	0.000 078
120 Hz	0.025	0.003 9	0.000 43	0.000 46	0.000 02	0.000 03	0.000 04	0.0000 4
125 Hz	0.025	0.003 9	0.000 43	0.000077	-	-	-	-
1 kHz	0.000 02	0.000 02	0.000 02	0.000 02	0.000 02	0.000 02	0.000 02	0.000 03
10 kHz	0.002 4	0.000 24	0.000 086	0.000 065	0.000 02	0.000 02	0.000 03	0.000 28
12.5 kHz	0.002 4	0.000 061	0.000 061	0.000 065	-	-	-	-
48 kHz	0.002 4	0.000 061	0.000 061	0.000 065	-	-	-	-
96 kHz	0.002 4	0.000 061	0.000 061	0.000 065	-	-	-	-
100 kHz	0.002 4	0.000 061	0.000 061	0.000 065	0.000 02	0.000 03	0.000 04	0.000 7
300 kHz	0.002 4	0.000 061	0.000 061	0.000 065	-	-	-	-
500 kHz	0.002 4	0.000 061	0.000 061	0.000 065	-	-	-	-
1 MHz	0.000 03	0.000 02	0.000 02	0.000 03	-	-	-	-
2 MHz	0.000 06	0.000 02	0.000 02	0.000 06	-	-	-	-
3 MHz	0.000 09	0.000 02	0.000 03	0.000 1	-	-	-	-
4 MHz	0.000 14	0.000 02	0.000 05	0.000 15	-	-	-	-
5 MHz	0.000 2	0.000 03	0.000 06	0.000 21	-	-	-	-
10 MHz	0.000 57	0.000 07	0.000 16	0.000 58	-	-	-	-
13 MHz	0.000 83	0.000 09	0.000 24	0.000 85	-	-	-	-

**Electrical – RF/Microwave**

**Main Scope**

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Attenuation – Measure Number of attenuation segments 1 or any configuration of multiple segments with attenuation totaling from 1 dB up to and including 40 dB	Type-N, 3.5 mm, 2.4 mm (1 to 40) dB (0.3 to 500) MHz (0.5 to 2) GHz (2 to 18) GHz (18 to 40) GHz (40 to 50) GHz	0.003 4 dB 0.004 7 dB $((0.011 \% \text{ of reading } * f) + 0.004 9) \text{ dB}$ 0.008 9 dB 0.012 dB	Comparison to a Keysight network analyzer
Attenuation – Measure Number of attenuation segments 2	Type-N: (50 to 80) dB 3.5 mm: 50, 60 dB 2.4 mm: 50 dB 300 kHz to 8 GHz (8 to 18) GHz (8 to 40) GHz (40 to 50) GHz	0.025 dB 0.029 dB 0.034 dB 0.037 dB	Comparison to a Keysight network analyzer
Attenuation – Measure Number of attenuation segments 3	Type-N: (70 to 100) dB 3.5 mm: 70 dB or 80 dB 300 kHz to 18 GHz (18 to 20) GHz (20 to 40) GHz (40 to 50) GHz	0.048 dB 0.056 dB 0.059 dB 0.065 dB	Comparison to a Keysight network analyzer
Attenuation – Measure Number of attenuation segments 4	Type-N: 110, 120 dB 3.5 mm: 90 dB 2.4 mm: 65 or 90 dB 300 kHz to 18 GHz (18 to 20) GHz (20 to 40) GHz (40 to 50) GHz	0.072 dB 0.08 dB 0.084 dB 0.094 dB	Comparison to a Keysight network analyzer
Attenuation – Measure	(1 to 12 dB) 20 Hz to 50 MHz 50 MHz to 1 GHz (1 to 2) GHz (2 to 4) GHz	0.002 4 dB 0.004 8 dB 0.005 8 dB 0.007 5 dB	Comparison to ratio transformer
RF Power - Measure DC VSWR <sup>1</sup>	1.0:1 to 2.0:1	0.000 32	Comparison to a Keysight 3458A multimeter
RF Power - Measure Calibration Factors <sup>1</sup> Absolute value	(0 to 105) % DC to 9 kHz	0.003 9	Comparison to a Keysight 3458A multimeter

**Electrical – RF/Microwave**

**Main Scope**

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
RF Power - Measure Calibration Factors <sup>1</sup> Absolute values	(0.5 to 1.5)		Comparison to a power sensor
	9 kHz to 30 kHz	0.003 1	
	30 kHz to 50 MHz	0.002 9	
	(50 to 100) MHz	0.002 1	
	(0.1 to 6) GHz	0.002 9	
	(6 to 7) GHz	0.003 1	
	(7 to 8) GHz	0.003 2	
	(8 to 18 GHz)	0.003 8	
	(18 to 26) GHz	0.008 1	
	(26 to 31) GHz	0.008 6	
	(31 to 37 GHz)	0.008 4	
	(37 to 38) GHz	0.009 3	
	(38 to 40) GHz	0.008 3	
	(40 to 46) GHz	0.014	
	(46 to 50) GHz	0.013	
	(50 to 67) GHz	0.02	
	(67 to 75) GHz	0.041	
(75 to 100) GHz	0.044		
(100 to 106) GHz	0.043		
(106 to 108) GHz	0.045		
(108 to 110) GHz	0.051		
(110 to 114) GHz	0.054		
(114 to 120) GHz	0.057		
RF Power - Measure Power Meter Reference	1 mW, 50 MHz	0.22 % of reading	Comparison to a power meter
RF Power - Measure (Relative)	(Ref -30 to 11 dBm)		Comparison to power sensors
	900 Hz to 9 kHz		
	(-40 to -35) dB	0.14 dB	
	(-35 to -30) dB	0.051 dB	
	(-30 to -3) dB	0.026 dB	
	(-3 to 3) dB	0.006 1 dB	
(3 to 10) dB	0.014 dB		
(10 to 30) dB	0.023 dB		



ANSI National Accreditation Board

Electrical – RF/Microwave

Main Scope

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
RF Power - Measure (Relative)	(Ref -30 to 11 dBm) 9 kHz to 50 GHz		
	(-130 to -110) dB	0.17 dB	
	(-110 to -100) dB		
	(9 to 100) kHz	0.064 dB	
	100 kHz to 3.6 GHz	0.05 dB	
	(3.6 to 30) GHz	0.07 dB	
	(30 to 50) GHz	0.074 dB	
	(-100 to -90) dB	0.044 dB	
	(-90 to -70) dB	0.034 dB	
	(-70 to -50) dB	0.029 dB	
	(-50 to -30) dB	0.018 dB	
	(-30 to -10) dB	0.009 2 dB	
	(-10 to -5) dB	0.006 5 dB	
	(-5 to 5) dB	0.002 2 dB	
	(5 to 10) dB	0.006 5 dB	
(10 to 20) dB	0.092 dB		
(20 to 30) dB	0.026 dB		
RF Power - Measure (Relative)	(Ref -30 to 11 dBm) (50 to 67) GHz		
	(-130 to -120) dB	0.22 dB	
	(-120 to -80) dB	0.17 dB	
	(-80 to -70) dB	0.21 dB	
	(-70 to -60) dB	0.050 dB	
	(-60 to -50) dB	0.033 dB	
	(-50 to -40) dB	0.025 dB	
	(-40 to -35) dB	0.021 dB	
	(-35 to -30) dB	0.019 dB	
	(-30 to -3) dB	0.005 6 dB	
	(-3 to 3) dB	0.002 2 dB	
	(3 to 10) dB	0.014 dB	
	(10 to 30) dB	0.023 dB	
	(67 to 110) GHz		
	(-40 to -35) dB	0.18 dB	
	(-35 to -30) dB	0.063 dB	
	(-30 to -3) dB	0.026 dB	
	(-3 to 3) dB	0.006 1 dB	
(3 to 10) dB	0.014 dB		
(10 to 30) dB	0.023 dB		
		Comparison to power sensors	



ANSI National Accreditation Board

Electrical – RF/Microwave

Main Scope

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
RF Power – Measure Relative	1 MHz to 2 GHz (Ref -10 to -20 dBm)		Comparison to a Keysight network analyzer, power sensor and signal source
	-60 dBm	0.004 9 dB	
	(-60 to 50) dBm	0.001 5 dB	
	(-50 to 40) dBm	0.000 84 dB	
	(-40 to 30) dBm	0.000 76 dB	
	(-30 to 20) dBm	0.000 23 dB	
	(-20 to 10) dBm	0.000 097 dB	
	(-10 to 5) dBm	0.000 11 dB	
	(-5 to 5) dBm	0.000 32 dB	
RF Power – Measure Relative	1.195 GHz (Ref -10 to -22 dBm)		Comparison to a Keysight network analyzer, power sensor and signal source
	(-80 to -79) dBm	0.041 dB	
	(-79 to -78) dBm	0.037 dB	
	(-78 to -77) dBm	0.035 dB	
	(-77 to -76) dBm	0.032 dB	
	(-76 to -75) dBm	0.03 dB	
	(-75 to -74) dBm	0.029 dB	
	(-74 to -73) dBm	0.028 dB	
	(-73 to -72) dBm	0.027 dB	
	(-72 to -70) dBm	0.026 dB	
	(-70 to -69) dBm	0.022 dB	
	(-69 to -67) dBm	0.021 dB	
	(-67 to -65) dBm	0.02 dB	
	(-65 to -60) dBm	0.019 dB	
	(-60 to -58) dBm	0.016 dB	
	(-58 to -54) dBm	0.015 dB	
	(-54 to -50) dBm	0.014 dB	
	(-50 to -49) dBm	0.013 dB	
	(-49 to -45) dBm	0.012 dB	
	(-45 to -40) dBm	0.011 dB	
	(-40 to -39) dBm	0.009 7 dB	
	(-39 to -38) dBm	0.009 1 dB	
	(-38 to -37) dBm	0.008 7 dB	
	(-37 to -35) dBm	0.008 2 dB	
(-35 to -31) dBm	0.007 9 dB		
(-31 to -30) dBm	0.007 8 dB		
(-30 to -29) dBm	0.006 6 dB		
(-29 to -28) dBm	0.005 7 dB		

**Electrical – RF/Microwave**

**Main Scope**

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
RF Power – Measure Relative	1.195 GHz (Ref -10 to -22 dBm) (-28 to -27) dBm (-27 to -26) dBm (-26 to -24) dBm (-24 to -21) dBm (-21 to 1) dBm (1 to 10) dBm	0.005 1 dB 0.004 6 dB 0.004 1 dB 0.003 8 dB 0.003 7 dB 0.005 3 dB	Comparison to a Keysight network analyzer, power sensor and signal source
RF Power – Measure Relative	1.998 77 GHz (Ref -20 dBm) (-60 to -57) dBm (-57 to -52) dBm (-52 to -49) dBm (-49 to -47) dBm (-47 to -46) dBm (-46 to -44) dBm (-44 to -42) dBm (-42 to -41) dBm (-41 to -39) dBm (-39 to -37) dBm (-37 to -35) dBm (-35 to -33) dBm (-33 to -31) dBm (-31 to -29) dBm (-29 to -27) dBm (-27 to -26) dBm (-26 to -25) dBm (-25 to -23) dBm (-23 to -22) dBm (-22 to -19) dBm (-19 to -14) dBm (-14 to -9) dBm (-9 to -4) dBm (-4 to 1) dBm (1 to 5) dBm	0.007 1 dB 0.006 7 dB 0.006 3 dB 0.006 dB 0.005 8 dB 0.005 4 dB 0.005 dB 0.004 8 dB 0.004 5 dB 0.004 1 dB 0.003 8 dB 0.003 5 dB 0.003 2 dB 0.003 dB 0.002 7 dB 0.002 5 dB 0.002 3 dB 0.001 9 dB 0.001 6 dB 0.001 dB 0.002 3 dB 0.003 3 dB 0.003 9 dB 0.004 7 dB 0.005 7 dB	Comparison to a Keysight network analyzer, power sensor and signal source

**Electrical – RF/Microwave**

**Main Scope**

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
RF Power Sensor - Linearity	50 MHz - 37 dBm (-36 to -30) dBm (-30 to -22) dBm (-22 to -15) dBm (-15 to -11) dBm (-11 to 0) dBm (0 to 9) dBm (9 to 13) dBm (13 to 18) dBm (18 to 21) dBm (21 to 26) dBm (26 to 30) dBm	0.39 % of reading 0.24 % of reading 0.0 % of reading 0.16 % of reading 0.12 % of reading 0.1 % of reading 0.061 % of reading 0.1 % of reading 0.11 % of reading 0.12 % of reading 0.33 % of reading 0.34 % of reading	Comparison to a Keysight network analyzer
Dynamic Range	(47 to 220 GHz) (80 to 130) dB	2.7 dB	Comparison to a Keysight network analyzer, millimeter wave test set
Amplitude Flatness - Measure	0.1 V to 8 V 100 kHz to 10 MHz (10 to 50) MHz 50 MHz (50 to 80) MHz 0.1 V to 5.5 V (80 to 300) MHz (0.3 to 1.1) GHz 0.01 V to 0.1 V (50 to 80) MHz (80 to 300) MHz (0.3 to 1.1) GHz	0.025 dB 0.028 dB 0.018 dB 0.023 dB 0.023 dB 0.033 dB 0.027 dB 0.032 dB 0.034 dB	Comparison to a power sensor, AC measurement standard and a Keysight 3458A multimeter
Amplitude Modulation Distortion - Measure	500 kHz to 50 GHz (0.01 to 0.1) % distortion (0.1 to 0.3) % distortion (0.3 to 15) % distortion	0.52% of reading + 0.001 1 % distortion 1% of reading + 0.000 63 % distortion 1.2 % distortion	Comparison to a signal analyzer

**Electrical – RF/Microwave**

**Main Scope**

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Frequency Modulation – Measure <sup>3</sup>	2 MHz to 3.6 GHz (0.2 to 100) (100 to 2 000)	0.35 % of reading + 0.2 % <i>M</i> 0.8 % <i>M</i>	Comparison to a signal analyzer
	(3.6 to 8.4) GHz (0.2 to 100) (100 to 2 000)	0.7 % of reading + 0.2 % <i>M</i> 2 % <i>M</i>	
	(8.4 to 17.1) GHz (0.2 to 100) (100 to 2 000)	0.7 % of reading + 0.3 % <i>M</i> 2.5 % <i>M</i>	
	(17.1 to 34.5) GHz (0.2 to 100) (100 to 2 000)	0.8 % of reading + 0.3 % <i>M</i> 3 % <i>M</i>	
	(34.5 to 50) GHz (0.2 to 100) (100 to 2 000)	1.4 % of reading + 0.5 % <i>M</i> 4 % <i>M</i>	
Frequency Modulation Distortion - Measure	500 kHz to 50 GHz (0.01 to 15) %	2.3 % distortion	Comparison to a Keysight signal analyzer
Phase Modulation Distortion - Measure	500 kHz to 50 GHz (0.01 to 15) %	2.3 % distortion	Comparison to a signal analyzer
Phase Modulation – Measure	(0.2 to 1) rad 100 kHz to 3.6 GHz (3.6 to 17.1) GHz (17.1 to 34.5) GHz (34.5 to 50) GHz	0.1% of reading + 0.001 rad 0.1% of reading + 0.002 rad 0.1% of reading + 0.002 5 rad 0.1% of reading + 0.004 9 rad	Comparison to a signal analyzer
	(1 to 10) rad 100 kHz to 3.6 GHz (3.6 to 17.1) GHz (17.1 to 34.5) GHz (34.5 to 50) GHz	0.008 1 % + 0.002 rad 0.015% of reading + 0.003 rad 0.02% of reading + 0.003 5 rad 0.058% of reading + 0.005 8 rad	
Phase Modulation Frequency Response - Measure	80 Hz to 100 kHz Deviation 4 rad	0.057 dB	Comparison to a signal analyzer and a Keysight 3458A multimeter
	100 Hz to 100 kHz Deviation 1 rad	0.14 dB	

**Electrical – RF/Microwave**

**Main Scope**

<b>Parameter/Equipment</b>	<b>Range</b>	<b>Expanded Uncertainty of Measurement (+/-)</b>	<b>Reference Standard, Method, and/or Equipment</b>
Digital Modulation – Measure GSM EDGE	(0.46 to 2.7) GHz EDGE: residual EVM (0 to 1.5) % EVM GSM: residual phase (0 to 1) ° GSM: peak phase (0 to 3) °	0.015 % EVM  0.01 °  0.12 °	Comparison to a signal analyzer
Digital Modulation – Measure CDMA2000 IS95 1xEV-DO	Residual EVM (0 to 2) % EVM (0.8 to 2.1) GHz	0.023 % EVM	Comparison to a signal analyzer
Digital Modulation – Measure W-CDMA	Residual EVM (0 to 2) % EVM (0.8 to 2.2) GHz	0.025 % EVM	Comparison to a signal analyzer
Digital Modulation – Measure BPSK	Residual EVM (0 to 2.5) % EVM ≤ 3 GHz (3 to 32) GHz (32 to 44) GHz	0.02 % EVM 0.055 % EVM 0.07 % EVM	Comparison to a signal analyzer
Digital Modulation – Measure QPSK	Residual EVM (0 to 2.5) % EVM ≤ 3 GHz (3 to 6) GHz (6 to 32) GHz (32 to 44) GHz	0.02 % EVM 0.026 % EVM 0.05 % EVM 0.065 % EVM	Comparison to a signal analyzer
Digital Modulation – Measure $\pi/4$ DQPSK	Residual EVM (0 to 2.5) % EVM ≤ 1 GHz (1 to 2) GHz (2 to 3) GHz (3 to 4) GHz (4 to 6) GHz	0.025 % EVM 0.046 % EVM 0.059 % EVM 0.11 % EVM 0.059 % EVM	Comparison to a signal analyzer
Digital Modulation – Measure 16, 64 and 256 QAM	Residual EVM (0 to 2.5) % EVM ≤ 3 GHz (3 to 6) GHz (6 to 32) GHz (32 to 44) GHz	0.015 % EVM 0.017 % EVM 0.03 % EVM 0.045 % EVM	Comparison to a Keysight signal analyzer

**Electrical – RF/Microwave**

**Main Scope**

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Digital Modulation – Measure 2FSK (including DECT)	Shift Error or Deviation (0 to 4.0) % EVM ≤ 3 GHz (3 to 6) GHz (0 to 10) kHz DECT – kHz	0.049 % EVM 0.048 % EVM  0.12 % of deviation	Comparison to a Keysight signal analyzer
Digital Modulation – Measure NADC	Residual EVM (0 to 2) % EVM (350 to 950) MHz	0.042 % EVM	Comparison to a Keysight signal analyzer
Digital Modulation – Measure PDC	Residual EVM (0 to 2) % EVM (350 to 1501) MHz	0.055 % EVM	Comparison to a Keysight signal analyzer
Digital Modulation – Measure PHS	Residual EVM (0 to 2) % EVM (0.35 to 2) GHz	0.035 % EVM	Comparison to a Keysight signal analyzer
Digital Modulation – Measure TETRA	Residual EVM (0 to 2) % EVM 350 MHz to 1 GHz	0.044 % EVM	Comparison to a Keysight signal analyzer
CISPR Quasi-Peak Absolute Amplitude	Band A, B, C	0.28 dB	Comparison to pulse generator
CISPR Quasi-Peak Detector Variation	Band A, B, C, D	0.12 dB	Comparison to pulse generator
CISPR Response to Pulses Peak Detector	Band A, B Band C, D	0.33 dB 0.3 dB	Comparison to pulse generator
CISPR Response to Pulses Average Detector	Band A Band B Band C, D	0.33 dB 0.35 dB 0.32 dB	Comparison to pulse generator
Distortion Measure	20 Hz to 20 kHz (20 to 100) kHz	1.2 dB 2.4 dB	Comparison to an audio analyzer
Excess Noise Ratio - Source	(5 to 22) dB (0.01 to 8) GHz (8 to 18) GHz (18 to 28) GHz (28 to 40) GHz (40 to 50) GHz	0.055 dB 0.035 dB 0.059 dB 0.078 dB 0.089 dB	Comparison to a noise source

**Electrical – RF/Microwave**

**Main Scope**

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Excess Noise Ratio - Measure Cold Source Method	(5 to 22) dB		Comparison to a Keysight network analyzer, and a power Sensor
	(0.5 to 6) GHz	0.1 dB	
	(6 to 18) GHz	0.11 dB	
	(18 to 26.5) GHz	0.13 dB	
	(26.5 to 33) GHz	0.14 dB	
	(33 to 36) GHz	0.15 dB	
	(36 to 39) GHz	0.16 dB	
	(39 to 40) GHz	0.17 dB	
	(40 to 48) GHz	0.2 dB	
	(48 to 50) GHz	0.21 dB	
	(50 to 60) GHz	0.27 dB	
	(60 to 64) GHz	0.29 dB	
(64 to 65) GHz	0.31 dB		
(65 to 67) GHz	0.29 dB		
Phase Noise – Measure	50 kHz to 54 GHz ≥ -187 dBc/Hz		Comparison to a phase noise measurement system
	≤ 10 Hz	2 dB	
	≤ 1 MHz	1.8 dB	
	≤ 100 MHz	3.6 dB	
Phase Noise – Source	1 GHz ≥ -167 dBc/Hz		Comparison to an ultra-low noise reference source
	(10 to 100) Hz	0.5 dB	
	(0.1 to 100) kHz	0.36 dB	
	(0.1 to 1) MHz	0.48 dB	
	(1 to 10) MHz	0.53 dB	
Phase Noise – Source	70 MHz to 1 GHz		Comparison to a low noise signal generator
	>-105 dBc/Hz	0.37 dB	
	>-120 dBc/Hz	0.37 dB	
	>-130 dBc/Hz	0.37 dB	
	>-130 dBc/Hz	0.4 dB	
>-145 dBc/Hz	0.4 dB		
Noise Voltage - Measure	20 MHz or 1 GHz peak to peak		Comparison to a differential amplifier and a voltmeter
	(>0 to 2) mV	0.07 mV	
	2 mV to 2 V	1.9 % of reading	
	20 MHz rms		
	(>0 to 0.5) mV	21 % of reading	
	(0.5 to 1) mV	6.6 % of reading	
1 mV to 1 V	1.9 % of reading		

**Electrical – RF/Microwave**

**Main Scope**

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Noise Current - Measure	20 MHz rms Up to 10 $\mu$ A (10 to 100) $\mu$ A (0.1 to 250) mA	33 mA/A + 5.7 $\mu$ A 0.11 A/A + 4.2 $\mu$ A 0.15 A/A	Comparison to an oscilloscope and a current probe

**Electrical – RF/Microwave**

**Main Scope**

Parameter/Equipment	Attenuation – Measure										
Reference Standard, Method, and/or Equipment	Comparison to a ratio transformer										
Expanded Uncertainty of Measurement (+/-) (in dB)											
Ranges	10 dB	20 dB	30 dB	40 dB	50 dB	60 dB	70 dB	80 dB	90 dB	100 dB	110 dB
20 Hz to 50 MHz	0.002 5 dB	0.003 5 dB	0.004 4 dB	0.006 7 dB	0.008 5 dB	0.01 dB	0.014 dB	0.017 dB	0.02 dB	0.03 dB	0.037 dB
50 MHz to 1 GHz	0.005 2 dB	0.007 4	0.009 1 dB	0.014 dB	0.017 dB	0.02 dB	0.029 dB	0.036 dB	0.042 dB	0.06 dB	0.074 dB
(1 to 2) GHz	0.006 6 dB	0.01 dB	0.012 dB	0.019 dB	0.024 dB	0.028 dB	0.04 dB	0.049 dB	0.057 dB	0.081 dB	0.1 dB
(2 to 4) GHz	0.006 8 dB	0.011 dB	0.015 dB	0.025 dB	0.031 dB	0.037 dB	0.053 dB	0.066 dB	0.077 dB	0.11 dB	0.13 dB

**Electrical – RF/Microwave**

**Main Scope**

Parameter/Equipment	Attenuation – Source										
Reference Standard, Method, and/or Equipment	Comparison to an attenuator										
Expanded Uncertainty of Measurement (+/-)											
Range	1 dB	2 dB	3 dB	4 dB	5 dB	6 dB	7 dB	8 dB	9 dB	10 dB	11 dB
20 Hz to 50 MHz	0.0028 dB	0.0028 dB	0.0028 dB	0.0029 dB	0.0029 dB	0.0029 dB	0.0029 dB	0.0029 dB	0.0029 dB	0.0029 dB	0.0029 dB
50 MHz to 1 GHz	0.0053 dB	0.0053 dB	0.0053 dB	0.0053 dB	0.0053 dB	0.0053 dB	0.0053 dB	0.0053 dB	0.0053 dB	0.0054 dB	0.0054 dB
(1 to 2) GHz	0.0063 dB	0.0063 dB	0.0063 dB	0.0063 dB	0.0063 dB	0.0063 dB	0.0063 dB	0.0063 dB	0.0063 dB	0.0063 dB	0.0063 dB
(2 to 4) GHz	0.008 dB	0.008 dB	0.0081 dB	0.0081 dB	0.0081 dB	0.0081 dB	0.0081 dB	0.0081 dB	0.0081 dB	0.0081 dB	0.0081 dB
(4 to 10) GHz	0.013 dB	0.012 dB	0.015 dB	0.014 dB	0.017 dB	0.016 dB	0.015 dB	0.015 dB	0.021 dB	0.013 dB	0.015 dB
(10 to 12.4) GHz	0.021 dB	0.027 dB	0.032 dB	0.027 dB	0.022 dB	0.022 dB	0.019 dB	0.024 dB	0.025 dB	0.036 dB	0.036 dB
(12.4 to 18) GHz	0.034 dB	0.037 dB	0.035 dB	0.033 dB	0.040 dB	0.038 dB	0.035 dB	0.038 dB	0.045 dB	0.042 dB	0.036 dB

**Electrical – RF/Microwave**

**Main Scope**

<b>Parameter/Equipment</b>	Attenuation – Source										
<b>Reference Standard, Method, and/or Equipment</b>	Comparison to an attenuator										
<b>Expanded Uncertainty of Measurement (+/-)</b>											
<b>Range</b>	10 dB	20 dB	30 dB	40 dB	50 dB	60 dB	70 dB	80 dB	90 dB	100 dB	110 dB
20 Hz to 50 MHz	0.0039 dB	0.0043 dB	0.0075 dB	0.0075 dB	0.0096 dB	0.011 dB	0.016 dB	0.019 dB	0.022 dB	0.032 dB	0.039 dB
50 MHz to 1 GHz	0.0051 dB	0.0048 dB	0.0057 dB	0.0065 dB	0.019 dB	0.022 dB	0.032 dB	0.039 dB	0.045 dB	0.057 dB	0.074 dB
(1 to 2) GHz	0.006 dB	0.0059 dB	0.006 dB	0.0083 dB	0.025 dB	0.029 dB	0.042 dB	0.033 dB	0.058 dB	0.058 dB	0.082 dB
(2 to 4) GHz	0.0075 dB	0.0073 dB	0.0082 dB	0.012 dB	0.034 dB	0.035 dB	0.057 dB	0.035 dB	0.06 dB	0.062 dB	0.086 dB
(4 to 10) GHz	0.01 dB	0.0098 dB	0.01 dB	0.012 dB	0.038 dB	0.038 dB	0.065 dB	0.038 dB	0.065 dB	0.068 dB	0.093 dB
(10 to 12.4) GHz	0.01 dB	0.0099 dB	0.01 dB	0.012 dB	0.038 dB	0.038 dB	0.065 dB	0.038 dB	0.065 dB	0.086 dB	0.12 dB
(12.4 to 18) GHz	0.01 dB	0.0099 dB	0.01 dB	0.012 dB	0.038 dB	0.038 dB	0.065 dB	0.038 dB	0.065 dB	0.17 dB	0.18 dB

**Electrical – RF/Microwave**

**Main Scope**

<b>Parameter/ Equipment</b>	RF Power - Measure											
<b>Reference Standard, Method, and/or Equipment</b>	Comparison to a power sensor and a signal analyzer											
<b>Expanded Uncertainty of Measurement (+/-)</b>												
<b>Range</b>	(-140 to -130) dBm	(-130 to -110) dBm	(-110 to -90) dBm	(-90 to -30) dBm	(-30 to -10) dBm	(-10 to -3) dBm	(-3 to +3) dBm	(3 to 14) dBm	(14 to 20) dBm	(20 to 25) dBm	(25 to 35) dBm	(35 to 44) dBm
(0.9 to 9) kHz	-	-	-	-	0.044 dB	0.044 dB	0.027 dB	0.032 dB	0.043 dB	-	-	-
(9 to 100) kHz	0.17 dB	0.17 dB	0.16 dB	0.16 dB	0.044 dB	0.044 dB	0.027 dB	0.032 dB	0.032 dB	0.034 dB	0.036 dB	-
(0.1 to 10) MHz	0.085 dB	0.071 dB	0.054 dB	0.045 dB	0.043 dB	0.042 dB	0.027 dB	0.032 dB	0.032 dB	0.034 dB	0.037 dB	-
50 MHz	0.079 dB	0.066 dB	0.048 dB	0.037 dB	0.034 dB	0.032 dB	0.02 dB	0.027 dB	0.023 dB	0.024 dB	0.029 dB	-
(10 to 100) MHz	0.081 dB	0.068 dB	0.05 dB	0.04 dB	0.038 dB	0.037 dB	0.027 dB	0.029 dB	0.032 dB	0.034 dB	0.036 dB	0.06 dB
(0.1 to 4) GHz	0.080 dB	0.067 dB	0.049 dB	0.039 dB	0.036 dB	0.035 dB	0.024 dB	0.027 dB	0.037 dB	0.038 dB	0.041 dB	0.057 dB
(4 to 8) GHz	0.081 dB	0.068 dB	0.05 dB	0.04 dB	0.038 dB	0.037 dB	0.027 dB	0.032 dB	0.039 dB	0.041 dB	0.043 dB	0.058 dB
(8 to 18) GHz	0.084 dB	0.071 dB	0.053 dB	0.043 dB	0.04 dB	0.039 dB	0.029 dB	0.035 dB	0.038 dB	0.04 dB	0.042 dB	0.06 dB
(18 to 24) GHz	0.091 dB	0.076 dB	0.069 dB	0.05 dB	0.048 dB	0.047 dB	0.031 dB	0.044 dB	0.053 dB	0.061 dB	0.063 dB	-
(24 to 40) GHz	0.12 dB	0.11 dB	0.1 dB	0.091 dB	0.069 dB	0.069 dB	0.059 dB	0.061 dB	0.068 dB	0.069 dB	0.076 dB	-
(40 to 50) GHz	0.13 dB	0.10 dB	0.098 dB	0.085 dB	0.083 dB	0.083 dB	0.079 dB	0.081 dB	0.086 dB	0.11 dB	0.11 dB	-
(50 to 60) GHz	0.17 dB	0.13 dB	0.12 dB	0.1 dB	0.099 dB	0.099 dB	0.093 dB	0.094 dB	0.099 dB	-	-	-
(60 to 67) GHz	0.52 dB	0.22 dB	0.22 dB	0.21 dB	0.099 dB	0.099 dB	0.093 dB	0.094 dB	0.099 dB	-	-	-
(67 to 80) GHz	-	-	-	-	0.26 dB	0.26 dB	0.26 dB	0.26 dB	0.26 dB	-	-	-

**Electrical – RF/Microwave**

**Main Scope**

<b>Parameter/ Equipment</b>		RF Power - Measure										
<b>Reference Standard, Method, and/or Equipment</b>		Comparison to a power sensor and a signal analyzer										
<b>Expanded Uncertainty of Measurement (+/-)</b>												
<b>Range</b>	(-140 to -130) dBm	(-130 to -110) dBm	(-110 to -90) dBm	(-90 to -30) dBm	(-30 to -10) dBm	(-10 to -3) dBm	(-3 to +3) dBm	(3 to 14) dBm	(14 to 20) dBm	(20 to 25) dBm	(25 to 35) dBm	(35 to 44) dBm
(80 to 90) GHz	-	-	-	-	0.32 dB	0.32 dB	0.32 dB	0.32 dB	0.32 dB	-	-	-
(90 to 100) GHz	-	-	-	-	0.3 dB	0.3 dB	0.3 dB	0.3 dB	0.3 dB	-	-	-
(100 to 110) GHz	-	-	-	-	0.29 dB	0.29 dB	0.29 dB	0.29 dB	0.29 dB	-	-	-

**Electrical – RF/Microwave**

**Main Scope**

<b>Parameter/Equipment</b>		Amplitude Modulation Depth - Measure		
<b>Reference Standard, Method, and/or Equipment</b>		Comparison to a signal analyzer (% indicates % depth where not specified)		
<b>Frequency Range</b>	<b>AM Depth</b>	<b>Modulation Rate</b>	<b>Expanded Uncertainty of Measurement (+/-)</b>	
2 Hz to 50 GHz	(5 to 20) %	10 Hz to 100 kHz	0.11% of reading + 0.0083 %	
	(20 to 40) %		0.022% of reading + 0.026 %	
	(40 to 50) %		0.0027% of reading + 0.034 %	
	(50 to 60) %		-0.013% of reading + 0.043 %	
	(60 to 75) %		-0.041% of reading + 0.06 %	
	(75 to 90) %		-0.091% of reading + 0.099 %	
	(90 to 95) %		0.01 %	
	(95 to 98) %		0.0051 %	
100 kHz to 13.6 GHz	(5 to 50) %	10 Hz to 25 kHz	0.1% of reading	
	(5 to 30) %	(25 to 50) kHz	0.16% of reading	
	(5 to 20) %	(50 to 100) kHz	0.22% of reading	
	(5 to 95) %	(100 to 250) kHz	0.32% of reading	
		(250 to 500) kHz	0.5% of reading	
		(0.5 to 1) MHz	0.71% of reading	
		1 MHz	1% of reading	

**Electrical – RF/Microwave**

**Main Scope**

Parameter/Equipment		Amplitude Modulation Depth - Measure		
Reference Standard, Method, and/or Equipment		Comparison to a signal analyzer (% indicates % depth where not specified)		
Frequency Range	AM Depth	Modulation Rate	Expanded Uncertainty of Measurement (+/-)	
(13.5 to 17.1) GHz	(5 to 50) %	10 Hz to 10 kHz	0.1% of reading	
	(5 to 35) %	(10 to 25) kHz	0.14% of reading	
	(5 to 20) %	(25 to 50) kHz	0.22% of reading	
	(5 to 15) %	(50 to 100) kHz	0.32% of reading	
	(5 to 95) %	(100 to 250) kHz	0.45% of reading	
		(250 to 500) kHz	0.71% of reading	
		(0.5 to 1) MHz	1% of reading	
1 MHz		1.4% of reading		
(17 to 34.5) GHz	(5 to 50) %	10 Hz to 5 kHz	0.1% of reading	
	(5 to 55) %	(5 to 10) kHz	0.095% of reading	
	(5 to 30) %	(10 to 25) kHz	0.15% of reading	
	(5 to 20) %	(25 to 50) kHz	0.25% of reading	
	(5 to 10) %	(50 to 100) kHz	0.36% of reading	
	(5 to 95) %	(100 to 250) kHz	0.52% of reading	
		(250 to 500) kHz	0.84% of reading	
		(0.5 to 1) MHz	1.2% of reading	
1 MHz		1.7% of reading		
(34.4 to 50) GHz	(5 to 15) %	10 Hz to 5 kHz	0.25% of reading	
	(5 to 15) %	(5 to 10) kHz	0.31% of reading	
	(5 to 10) %	(10 to 25) kHz	0.37% of reading	
	(5 to 95) %	(100 to 250) kHz	1.5% of reading	
		(250 to 500) kHz	3.3% of reading	
		(0.5 to 1) MHz	6.3% of reading	
		1 MHz	12% of reading	

**Electrical – RF/Microwave**

**Main Scope**

Parameter/Equipment		Frequency Modulation Deviation - Measure		
Reference Standard, Method, and/or Equipment		Comparison to a signal analyzer		
Frequencies	Deviation Range	Modulation Rate	Modulation index	Expanded Uncertainty of Measurement (+/-)
100 kHz to 3.6 GHz	20 Hz to 2 MHz	10 Hz to 500 kHz	$\beta \geq 0.5$	0.2 % Deviation
100 kHz to 3.6 GHz	10 Hz to 10 MHz	20 Hz to 1 MHz	$\beta \geq 0.2$	0.7 % Deviation
100 kHz to 3.6 GHz	10 Hz to 16 MHz	50 Hz to 1 MHz	$\beta \geq 0.05$	2 % Deviation

**Electrical – RF/Microwave**

**Main Scope**

Parameter/Equipment		Frequency Modulation Deviation - Measure		
Reference Standard, Method, and/or Equipment		Comparison to a signal analyzer		
Frequencies	Deviation Range	Modulation Rate	Modulation index	Expanded Uncertainty of Measurement (+/-)
100 kHz to 3.6 GHz	10 Hz to 50 kHz	100 Hz to 1 MHz	$\beta \geq 0.025$	5.2 % Deviation
100 kHz to 3.6 GHz	10 Hz to 40 kHz	100 Hz to 1 MHz	$\beta \geq 0.02$	10 % Deviation
100 kHz to 3.6 GHz	10 Hz to 20 kHz	500 Hz to 1 MHz	$\beta \geq 0.01$	20 % Deviation
(3.5 to 8.4) GHz	20 Hz to 1 MHz	10 Hz to 500 kHz	$\beta \geq 0.5$	0.21 % Deviation
(3.5 to 8.4) GHz	10 Hz to 5 MHz	20 Hz to 1 MHz	$\beta \geq 0.2$	0.7 % Deviation
(3.5 to 8.4) GHz	10 Hz to 16 MHz	50 Hz to 1 MHz	$\beta \geq 0.05$	2.2 % Deviation
(3.5 to 8.4) GHz	10 Hz to 16 MHz	100 Hz to 1 MHz	$\beta \geq 0.025$	5.2 % Deviation
(3.5 to 8.4) GHz	10 Hz to 40 kHz	100 Hz to 1 MHz	$\beta \geq 0.02$	10 % Deviation
(3.5 to 8.4) GHz	10 Hz to 20 kHz	500 Hz to 1 MHz	$\beta \geq 0.01$	20 % Deviation
(8.3 to 13.6) GHz	20 Hz to 2 MHz	10 Hz to 500 kHz	$\beta \geq 0.5$	0.21 % Deviation
(8.3 to 13.6) GHz	10 Hz to 10 MHz	50 Hz to 1 MHz	$\beta \geq 0.2$	0.7 % Deviation
(8.3 to 13.6) GHz	10 Hz to 16 MHz	50 Hz to 1 MHz	$\beta \geq 0.05$	2.2 % Deviation
(8.3 to 13.6) GHz	10 Hz to 500 kHz	100 Hz to 1 MHz	$\beta \geq 0.025$	5.2 % Deviation
(8.3 to 13.6) GHz	10 Hz to 40 kHz	100 Hz to 1 MHz	$\beta \geq 0.02$	10 % Deviation
(8.3 to 13.6) GHz	10 Hz to 20 kHz	500 Hz to 1 MHz	$\beta \geq 0.01$	20 % Deviation
(13.5 to 17.1) GHz	20 Hz to 1 MHz	10 Hz to 200 kHz	$\beta \geq 0.5$	0.21 % Deviation
(13.5 to 17.1) GHz	10 Hz to 5 MHz	20 Hz to 1 MHz	$\beta \geq 0.2$	0.7 % Deviation
(13.5 to 17.1) GHz	10 Hz to 16 MHz	50 Hz to 1 MHz	$\beta \geq 0.05$	2.2 % Deviation
(13.5 to 17.1) GHz	10 Hz to 16 MHz	100 Hz to 1 MHz	$\beta \geq 0.025$	5.2 % Deviation
(13.5 to 17.1) GHz	10 Hz to 40 kHz	100 Hz to 1 MHz	$\beta \geq 0.02$	10 % Deviation
(13.5 to 17.1) GHz	10 Hz to 20 kHz	500 Hz to 1 MHz	$\beta \geq 0.01$	20 % Deviation
(17 to 26.5) GHz	50 Hz to 400 kHz	10 Hz to 50 kHz	$\beta \geq 0.8$	0.31 % Deviation
(17 to 26.5) GHz	20 Hz to 5 MHz	10 Hz to 1 MHz	$\beta \geq 0.2$	0.9 % Deviation
(17 to 26.5) GHz	20 Hz to 10 MHz	100 Hz to 1 MHz	$\beta \geq 0.08$	3.3 % Deviation
(17 to 26.5) GHz	10 Hz to 16 MHz	100 Hz to 1 MHz	$\beta \geq 0.04$	6.3 % Deviation
(17 to 26.5) GHz	10 Hz to 40 kHz	100 Hz to 1 MHz	$\beta \geq 0.02$	12 % Deviation
(17 to 26.5) GHz	10 Hz to 1 kHz	500 Hz to 100 kHz	$\beta \geq 0.01$	30 % Deviation
(26.4 to 34.5) GHz	50 Hz to 400 kHz	10 Hz to 50 kHz	$\beta \geq 0.8$	0.31 % Deviation
(26.4 to 34.5) GHz	20 Hz to 5 MHz	10 Hz to MHz	$\beta \geq 0.2$	0.9 % Deviation
(26.4 to 34.5) GHz	20 Hz to 10 MHz	100 Hz to 1 MHz	$\beta \geq 0.08$	3.3 % Deviation
(26.4 to 34.5) GHz	10 Hz to 16 MHz	100 Hz to 1 MHz	$\beta \geq 0.04$	6.3 % Deviation

**Electrical – RF/Microwave**

**Main Scope**

<b>Parameter/Equipment</b>		Frequency Modulation Deviation - Measure		
<b>Reference Standard, Method, and/or Equipment</b>		Comparison to a signal analyzer		
<b>Frequencies</b>	<b>Deviation Range</b>	<b>Modulation Rate</b>	<b>Modulation index</b>	<b>Expanded Uncertainty of Measurement (+/-)</b>
(26.4 to 34.5) GHz	10 Hz to 16 MHz	100 Hz to 1 MHz	$\beta \geq 0.02$	12 % Deviation
(26.4 to 34.5) GHz	10 Hz to 1 kHz	500 Hz to 100 kHz	$\beta \geq 0.01$	30 % Deviation
(34.4 to 50) GHz	50 Hz to 100 kHz	10 Hz to 20 kHz	$\beta \geq 0.8$	0.32 % Deviation
(34.4 to 50) GHz	20 Hz to 500 kHz	10 Hz to 200 kHz	$\beta \geq 0.2$	0.9 % Deviation
(34.4 to 50) GHz	20 Hz to 2 MHz	20 Hz to 1 MHz	$\beta \geq 0.08$	3.3 % Deviation
(34.4 to 50) GHz	10 Hz to 5 MHz	50 Hz to 1 MHz	$\beta \geq 0.04$	6.4 % Deviation
(34.4 to 50) GHz	10 Hz to 16 MHz	100 Hz to 1 MHz	$\beta \geq 0.02$	12 % Deviation
(34.4 to 50) GHz	10 Hz to 16 MHz	500 Hz to 200 kHz	$\beta \geq 0.01$	30 % Deviation

**Electrical - RF Microwave**

**Main Scope**

<b>Parameter/Equipment</b>		Voltage Reflection Coefficient S11/S22 - Magnitude (Linear)								
<b>Reference Standard, Method, and/or Equipment</b>		Comparison to a Keysight network analyzer								
<b>Expanded Uncertainty of Measurement (+/-)</b>										
<b>Range</b>	0 to 0.1	0.1 to 0.2	0.2 to 0.3	0.3 to 0.4	0.4 to 0.5	0.5 to 0.6	0.6 to 0.7	0.7 to 0.8	0.8 to 0.9	0.9 to 1.0
DC to 10 MHz	0.000 17	0.000 23	0.000 3	0.000 37	0.000 41	0.000 45	0.000 48	0.000 51	0.000 53	0.000 22
10 MHz to 2 GHz	0.000 18	0.000 23	0.000 31	0.000 38	0.000 43	0.000 47	0.000 5	0.000 52	0.000 53	0.000 22
(2 to 8) GHz	0.000 56	0.000 61	0.000 71	0.000 76	0.000 75	0.000 72	0.000 66	0.000 59	0.000 55	0.000 23
(8.0 to 20) GHz	0.000 56	0.000 61	0.000 7	0.000 8	0.000 9	0.001	0.000 97	0.000 94	0.000 94	0.000 89
(20 to 26.5) GHz	0.000 89	0.000 96	0.001 1	0.001 2	0.001 4	0.001 6	0.001 5	0.001 4	0.001 4	0.001 4
(26.5 to 33) GHz	0.000 89	0.000 98	0.001 2	0.001 4	0.001 7	0.001 8	0.001 6	0.001 5	0.001 4	0.001 4
(33 to 40) GHz	0.000 9	0.000 99	0.001 2	0.001 5	0.001 7	0.002	0.001 8	0.001 6	0.001 5	0.001 5
(40 to 45) GHz	0.001 4	0.001 5	0.001 7	0.001 9	0.002 1	0.002 4	0.002 3	0.002 1	0.002 1	0.002 1
(45 to 50) GHz	0.001 4	0.001 5	0.001 7	0.001 8	0.002	0.002 2	0.002 4	0.002 3	0.002 1	0.002 1
(50 to 60) GHz	0.002 5	0.002 6	0.002 8	0.003 1	0.003 4	0.003 7	0.004	0.004 3	0.004 7	0.005 3
(60 to 67) GHz	0.002 5	0.002 7	0.002 9	0.003 2	0.003 7	0.004 2	0.004 7	0.005 1	0.005 7	0.006 4
(67 to 75) GHz	0.005 4	0.005 9	0.006 1	0.006 3	0.006 5	0.006 8	0.007 1	0.007 5	0.007 8	0.008 2
(75 to 110) GHz	0.003 5	0.004	0.004 2	0.004 6	0.004 9	0.005 3	0.005 8	0.006 3	0.006 9	0.007 5
(110 to 120) GHz	0.03	0.033	0.036	0.039	0.04	0.047	0.052	0.057	0.063	0.07

**Electrical - RF Microwave**

**Main Scope**

Parameter/Equipment	Voltage Reflection Coefficient S11/S22 – Phase									
Reference Standard, Method, and/or Equipment	Comparison to a Keysight network analyzer									
Expanded Uncertainty of Measurement (+/-)										
Range	0 to 0.1	0.1 to 0.2	0.2 to 0.3	0.3 to 0.4	0.4 to 0.5	0.5 to 0.6	0.6 to 0.7	0.7 to 0.8	0.8 to 0.9	0.9 to 1.0
DC to 10 MHz	0.13°	0.086°	0.070°	0.059°	0.052°	0.046°	0.041°	0.038°	0.035°	0.013°
10 MHz to 2 GHz	0.13°	0.089°	0.073°	0.062°	0.054°	0.048°	0.043°	0.038°	0.035°	0.013°
(2.0 to 8.0) GHz	0.37°	0.22°	0.16°	0.12°	0.094°	0.076°	0.063°	0.05°	0.042°	0.026°
(8.0 to 20) GHz	0.39°	0.26°	0.21°	0.16°	0.13°	0.11°	0.092°	0.081°	0.071°	0.065°
(20 to 26.5) GHz	0.58°	0.40°	0.36°	0.29°	0.23°	0.2°	0.17°	0.16°	0.15°	0.15°
(26.5 to 33) GHz	0.57°	0.36°	0.31°	0.0°	0.29°	0.23°	0.19°	0.16°	0.14°	0.14°
(33 to 40) GHz	0.58°	0.39°	0.34°	0.32°	0.29°	0.24°	0.19°	0.16°	0.14°	0.13°
(40 to 45) GHz	0.86°	0.50°	0.39°	0.34°	0.32°	0.31°	0.31°	0.27°	0.26°	0.26°
(45 to 50) GHz	0.88°	0.55°	0.46°	0.43°	0.42°	0.36°	0.31°	0.28°	0.26°	0.26°
(50 to 60) GHz	1.5°	0.82°	0.63°	0.55°	0.52°	0.51°	0.52°	0.53°	0.5°	0.47°
(60 to 67) GHz	1.5°	0.84°	0.65°	0.58°	0.55°	0.54°	0.54°	0.53°	0.5°	0.47°
(67 to 75) GHz	3.2°	1.7°	1.2°	0.90°	0.75°	0.65°	0.58°	0.53°	0.5°	0.47°
(75 to 110) GHz	2.1°	1.1°	0.81°	0.65°	0.57°	0.51°	0.48°	0.45°	0.44°	0.43°
(110 to 120) GHz	18°	9.6°	6.9°	5.6°	4.9°	4.5°	4.3°	4.1°	4.0°	4.0°

**Electrical - RF Microwave**

**Main Scope**

Parameter/Equipment	Transmission S12/S21 – Magnitude								
Reference Standard, Method, and/or Equipment	Comparison to a Keysight network analyzer								
Expanded Uncertainty of Measurement (+/-)									
Range	(0 to 3) dB	(3 to 6) dB	(6 to 10) dB	(10 to 20) dB	(20 to 30) dB	(30 to 40) dB	(40 to 50) dB	(50 to 60) dB	(60 to 70) dB
DC to 10 MHz	0.000 57 dB	0.005 8 dB	0.007 3 dB	0.009 3 dB	0.013 dB	0.017 dB	0.02 dB	0.026 dB	0.044 dB
10 MHz to 2 GHz	0.000 3 dB	0.005 3 dB	0.006 1 dB	0.007 2 dB	0.01 dB	0.014 dB	0.017 dB	0.021 dB	0.028 dB
(2.0 to 8.0) GHz	0.000 3 dB	0.005 3 dB	0.006 1 dB	0.007 2 dB	0.01 dB	0.014 dB	0.017 dB	0.021 dB	0.028 dB
(8.0 to 20) GHz	0.000 3 dB	0.005 3 dB	0.006 1 dB	0.007 2 dB	0.01 dB	0.015 dB	0.018 dB	0.021 dB	0.026 dB
(20 to 26.5) GHz	0.009 3 dB	0.01 dB	0.011 dB	0.012 dB	0.014 dB	0.016 dB	0.019 dB	0.022 dB	0.027 dB
(26.5 to 33) GHz	0.014 3 dB	0.015 dB	0.015 dB	0.016 dB	0.017 dB	0.019 dB	0.022 dB	0.028 dB	0.051 dB
(33 to 40) GHz	0.020 1 dB	0.021 dB	0.021 dB	0.021 dB	0.022 dB	0.026 dB	0.031 dB	0.036 dB	0.056 dB

**Electrical - RF Microwave**

**Main Scope**

<b>Parameter/Equipment</b>	Transmission S12/S21 – Magnitude								
<b>Reference Standard, Method, and/or Equipment</b>	Comparison to a Keysight network analyzer								
<b>Expanded Uncertainty of Measurement (+/-)</b>									
<b>Range</b>	(0 to 3) dB	(3 to 6) dB	(6 to 10) dB	(10 to 20) dB	(20 to 30) dB	(30 to 40) dB	(40 to 50) dB	(50 to 60) dB	(60 to 70) dB
(40 to 45) GHz	0.022 dB	0.022 dB	0.023 dB	0.023 dB	0.024 dB	0.028 dB	0.037 dB	0.044 dB	0.08 dB
(45 to 50) GHz	0.023 1 dB	0.024 dB	0.024 dB	0.024 dB	0.025 dB	0.029 dB	0.037 dB	0.045 dB	0.08 dB
(50 to 60) GHz	0.027 9 dB	0.028 dB	0.028 dB	0.029 dB	0.03 dB	0.031 dB	0.033 dB	0.042 dB	0.085 dB
(60 to 67) GHz	0.034 dB	0.034 dB	0.034 dB	0.035 dB	0.035 dB	0.037 dB	0.039 dB	0.048 dB	0.096 dB
(67 to 75) GHz	0.043 dB	0.046 dB	0.048 dB	0.051 dB	0.057 dB	0.064 dB	0.071 dB	0.078 dB	0.088 dB
(75 to 100) GHz	0.038 dB	0.041 dB	0.044 dB	0.046 dB	0.053 dB	0.06 dB	0.067 dB	0.074 dB	0.084 dB
(100 to 110) GHz	0.044 dB	0.048 dB	0.051 dB	0.054 dB	0.061 dB	0.068 dB	0.075 dB	0.082 dB	0.098 dB
(110 to 120) GHz	0.44 dB	0.44 dB	0.44 dB	0.44 dB	0.45 dB	0.45 dB	0.46 dB	0.47 dB	0.48 dB

**Electrical - RF Microwave**

**Main Scope**

<b>Parameter/Equipment</b>	Transmission S12/S21 - Phase								
<b>Reference Standard, Method, and/or Equipment</b>	Comparison to Keysight network analyzer								
<b>Expanded Uncertainty of Measurement (+/-)</b>									
<b>Range</b>	(0 to 3) dB	(3 to 6) dB	(6 to 10) dB	(10 to 20) dB	(20 to 30) dB	(30 to 40) dB	(40 to 50) dB	(50 to 60) dB	(60 to 70) dB
DC to 10 MHz	0.004 3°	0.039°	0.048°	0.061°	0.084°	0.006 2°	0.007 9°	0.008 2°	0.008 5°
10 MHz to 2 GHz	0.002 9°	0.035°	0.04°	0.048°	0.067°	0.0062°	0.007 8°	0.007 9°	0.008 1°
(2 to 8) GHz	0.002 9°	0.035°	0.0°	0.048°	0.067°	0.006 8°	0.008 2°	0.008 4°	0.008 5°
(8 to 20) GHz	0.032°	0.035°	0.04°	0.048°	0.067°	0.00 91°	0.01°	0.01°	0.01°
(20 to 26.5) GHz	0.15°	0.15°	0.15°	0.15°	0.16°	0.011°	0.012°	0.012°	0.012°
(26.5 to 33) GHz	0.18°	0.18°	0.19°	0.19°	0.19°	0.015°	0.016°	0.016°	0.016°
(33 to 40) GHz	0.23°	0.24°	0.24°	0.24°	0.24°	0.25°	0.26°	0.28°	0.4°
(40 to 45) GHz	0.29°	0.29°	0.29°	0.29°	0.3°	0.31°	0.32°	0.35°	0.56°
(45 to 50) GHz	0.31°	0.31°	0.31°	0.31°	0.32°	0.32°	0.33°	0.37°	0.57°
(50 to 60) GHz	0.28°	0.38°	0.38°	0.38°	0.38°	0.39°	0.4°	0.43°	0.65°
(60 to 67) GHz	0.28°	0.43°	0.43°	0.43°	0.44°	0.44°	0.45°	0.49°	0.73°
(50 to 75) GHz	0.28°	0.3°	0.32°	0.34°	0.38°	0.42°	0.47°	0.52°	0.58°
(75 to 100) GHz	0.25°	0.27°	0.29°	0.31°	0.35°	0.4°	0.44°	0.49°	0.56°
(100 to 110) GHz	0.29°	0.32°	0.34°	0.36	0.4°	0.45°	0.49°	0.55°	0.65°
(110 to 120) GHz	3°	3°	3°	3°	3°	3.1°	3.1°	3.2°	3.3°

**Electrical – RF/Microwave**

**Main Scope**

Parameter/Equipment		Impedance – Source and Measure						
Reference Standard, Method, and/or Equipment		Comparison to a performance test kit						
Expanded Uncertainty of Measurement (+/-)								
Range	Admittance Open Magnitude 3 $\mu$ S to 15 mS	Impedance Short Magnitude 0 $\Omega$	Impedance Load Magnitude 50 $\Omega$	Impedance Load Phase (-1 to 1) $^\circ$	Impedance Airline Short Magnitude (0 to 25) $\Omega$	Impedance Airline Short Phase (-100 to 100) $^\circ$	Impedance Airline Open Magnitude 50 $\Omega$ to 25 k $\Omega$	Impedance Airline Open Phase (-100 to 100) $^\circ$
1 kHz	-	-	0.05 $\Omega$	0.095 mrad	-	-	-	-
1 MHz	0.18 $\mu$ S	2.5 m $\Omega$	0.08 $\Omega$	1.6 mrad	0.000 23 $\Omega$	2.1 mrad	39 $\Omega$	1.8 mrad
10 MHz	0.21 $\mu$ S	3.5 m $\Omega$	0.079 $\Omega$	1.6 mrad	0.002 2 $\Omega$	2.1 mrad	3.9 $\Omega$	1.8 mrad
100 MHz	2.1 $\mu$ S	14 m $\Omega$	0.077 $\Omega$	1.5 mrad	0.023 $\Omega$	2.2 mrad	0.38 $\Omega$	1.8 mrad
200 MHz	6.9 $\mu$ S	25 m $\Omega$	0.12 $\Omega$	2.3 mrad	0.053 $\Omega$	2.4 mrad	0.22 $\Omega$	2.2 mrad
300 MHz	10 $\mu$ S	30 m $\Omega$	0.12 $\Omega$	2.3 mrad	0.087 $\Omega$	2.4 mrad	0.13 $\Omega$	2.2 mrad
500 MHz	17 $\mu$ S	40 m $\Omega$	0.16 $\Omega$	3.2 mrad	0.29 $\Omega$	3.4 mrad	0.072 $\Omega$	3.2 mrad
600 MHz	20 $\mu$ S	40 m $\Omega$	0.21 $\Omega$	4.2 mrad	0.72 $\Omega$	4.6 mrad	0.053 $\Omega$	5.4 mrad
800 MHz	27 $\mu$ S	50 m $\Omega$	0.22 $\Omega$	4.5 mrad	0.45 $\Omega$	5.3 mrad	0.077 $\Omega$	5.6 mrad
1 GHz	33 $\mu$ S	50 m $\Omega$	0.25 $\Omega$	5 mrad	0.14 $\Omega$	6.3 mrad	0.24 $\Omega$	5.4 mrad
1.3 GHz	43 $\mu$ S	100 m $\Omega$	0.3 $\Omega$	6 mrad	0.092 $\Omega$	8.4 mrad	-	-
1.6 GHz	59 $\mu$ S	100 m $\Omega$	0.35 $\Omega$	7 mrad	0.28 $\Omega$	7.5 mrad	0.62 $\Omega$	7.2 mrad
1.8 GHz	68 $\mu$ S	100 m $\Omega$	0.36 $\Omega$	7.3 mrad	0.92 $\Omega$	10 mrad	0.25 $\Omega$	7.5 mrad
2 GHz	85 $\mu$ S	200 m $\Omega$	0.5 $\Omega$	10 mrad	1.7 $\Omega$	11 mrad	0.08 $\Omega$	12 mrad
2.2 GHz	95 $\mu$ S	200 m $\Omega$	0.49 $\Omega$	9.8 mrad	0.58 $\Omega$	11 mrad	0.18 $\Omega$	11 mrad
2.4 GHz	110 $\mu$ S	200 m $\Omega$	0.47 $\Omega$	9.3 mrad	0.23 $\Omega$	11 mrad	0.53 $\Omega$	10 mrad
2.6 GHz	130 $\mu$ S	200 m $\Omega$	0.43 $\Omega$	8.7 mrad	0.000 23 $\Omega$	2.1 mrad	2.1 $\Omega$	14 mrad
2.8 GHz	140 $\mu$ S	200 m $\Omega$	0.41 $\Omega$	8.2 mrad	0.002 2 $\Omega$	2.1 mrad	-	-
3 GHz	160 $\mu$ S	200 m $\Omega$	0.42 $\Omega$	8.4 mrad	-	-	1.1 $\Omega$	15 mrad

**Length – Dimensional Metrology**

**Main Scope**

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Digital Indicators <sup>2</sup>	Up to 100 mm	0.002 1 mm	Comparison to gage blocks
Dial Indicators <sup>2</sup>	Up to 100 mm	0.003 4 mm	Comparison to gage blocks

**Length – Dimensional Metrology**

**Main Scope**

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Feeler Gage <sup>2</sup>	(0.03 to 8.00) mm	0.001 1 mm	Comparison to a micrometer
Calipers <sup>2</sup>	Up to 300 mm	10 μm	Comparison to caliper checker
Micrometers <sup>2</sup>	Up to 25 mm	1 μm	Comparison to gage blocks
Plain Plug Gages and Pin Gages, Diameter <sup>2</sup>	Up to 25 mm	0.59 μm	Comparison to a supermicrometer, laser interferometer, master cylinder gage
Thread Plug Gages Pitch Diameter <sup>2</sup>	Up to 25 mm	0.001 5 mm	Comparison to a supermicrometer, laser interferometer, master cylinder gage and thread wire

**Mass and Mass Related**

**Main Scope**

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Electric Torque Screwdriver <sup>2</sup>	(1 to 1.77) lbf·in (1.78 to 16) lbf·in (16 to 43.4) lbf·in	0.03 lbf·in 0.1 lbf·in (0.006 5τ + 0.009 1) lbf·in	Comparison to a torque analyzer
Torque – Measure	(4 to 50) lbf·in	0.7% of reading	Comparison to a torque analyzer
Pressure – Source and Measure	(70 to 110) kPa	0.02 kPa	Comparison to a pressure monitor

**Mass and Mass Related**

**Main Scope**

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Scales and Balances <sup>2,4</sup>	(5 to 500) mg	0.015 mg	Comparison to reference mass standards
	(0.5 to 5) g	0.041 mg	
	(5 to 10) g	0.078 mg	
	(10 to 20) g	0.1 mg	
	(20 to 50) g	0.13 mg	
	(50 to 100) g	0.21 mg	
	(100 to 200) g	0.39 mg	
	(200 to 300) g	0.59 mg	
	(300 to 500) g	1 mg	
(500 to 600) g	1.2 mg		

**Photometry and Radiometry**

**Main Scope**

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Laser Optical Power – Measure	(80 to 1 000) $\mu$ W (488 to 788) nm	0.046 $\mu$ W/W + 0.09 $\mu$ W	Comparison to photodiode power sensor
Laser Wavelength - Measure	633 nm	0.000 0045 nm	Comparison to laser head

**Thermodynamic**

**Main Scope**

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Temperature – Source and Measure	(-1 to 41) °C (18 to 28) °C	0.01 °C	Comparison to reference thermometer
		0.005 °C	
Temperature – Source <sup>2</sup>	(5 to 55) °C	0.04 °C	Comparison to a humidity calibrator and a PRT
Temperature – Measure <sup>2</sup>	(-197 to 0) °C (0 to 200) °C (200 to 420) °C (420 to 660) °C	0.01 °C	Comparison to a PRT and a temperature scanner
		0.016 °C	
		0.026 °C	
		0.039 °C	
Humidity – Source and Measure	(5 to 95) %RH	0.8 %RH	Comparison to humidity generator
Humidity – Source	(20 to 80) %RH	1.3 %RH	Comparison to temperature and humidity calibrator and a thermohygrometer

**Time and Frequency**

**Main Scope**

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Frequency – Source	10 MHz	0.39 pHz/Hz	Comparison to Cesium frequency standard
Frequency – Source	10 MHz	1.2 pHz/Hz	Comparison to GPS frequency standard
Frequency – Source	10 MHz	510 pHz/Hz	Comparison to Rubidium frequency standard
Frequency – Source	(0.1 to 1) Hz 1 Hz to 250 kHz 250 kHz to 1 MHz 1 MHz to 12.4 GHz (12.4 to 46) GHz	2.0 $\mu$ Hz/Hz + 0.4 $\mu$ Hz 2.4 $\mu$ Hz/Hz 5.1 nHz/Hz + 0.13 mHz 5.2 nHz/Hz 5.2 nHz/Hz + 2 $\mu$ Hz	Comparison to Rubidium frequency standard and a function generator
Frequency – Measure	(0.1 to 1) Hz (1 to 10) Hz (10 to 100) Hz 100 Hz to 1 kHz (1 to 100) kHz 100 kHz to 10 MHz 10 MHz to 12.4 GHz (12.4 to 46) GHz	1.2 pHz/Hz + 63 pHz 0.61 pHz/Hz + 0.85 pHz 4.5 pHz/Hz + 4.1 nHz 23 pHz/Hz + 22 pHz 23 pHz/Hz + 0.13 nH 23 pHz/Hz + 33 nHz 23 pHz/Hz + 32 nHz 24 pHz/Hz + 1.1 Hz	Comparison to frequency counter
Time Interval – Measure	10 ps to 430 ps 430 ps to 1 $\mu$ s 1 $\mu$ s to 50 ms 50 ms to 1 s 1 s to 10 s 10 s to 100 s	12 ms/s + 1.2 ps 6.7 ps 36 ns/s + 7.5 ps 1.9 ns 26 ps/s + 2.1 ns 33 ps/s + 2.7 ns	Comparison to a frequency counter and an oscilloscope
Transition - Measure	(8 to 30) ps (30 to 50) ps (50 to 200) ps (200 to 500) ps	1.2 ps 1.3 ps 10 fs/s + 0.9 ps 9.4 fs/s + 1 ps	Comparison to an oscilloscope


**Time and Frequency**

**Main Scope**

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Jitter - Source	(0.01 to 25) ps 2 GHz 2.5 GHz 2.75 GHz 3 GHz 3.2 GHz 5 GHz 8 GHz 10 GHz 12 GHz 13 GHz 14 GHz 15 GHz 28 GHz 32 GHz	0.12 ps 44 fs 65 fs 0.13 ps 0.13 ps 0.1 ps 52 fs 31 fs 50 fs 50 fs 0.1 ps 50 fs 42 fs 37 fs	Comparison to a signal generator
Jitter - Measure	(0.1 to 130) ps 200 kHz to 15 GHz	1.9 ps	Comparison to an oscilloscope

[Return to Site listing \(top\)](#)

[Go to Notes \(bottom\)](#)

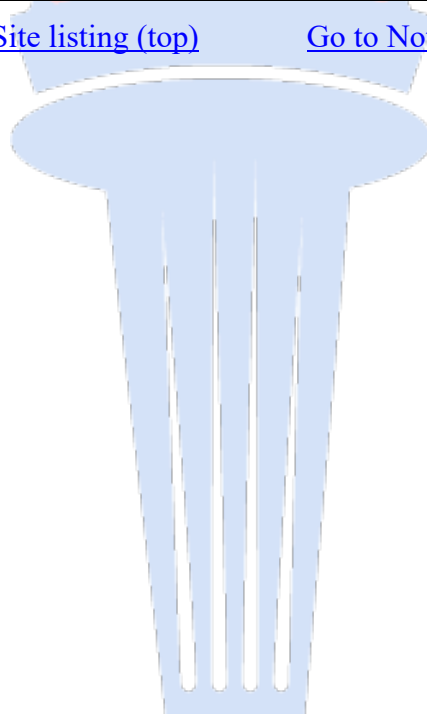



ANSI National Accreditation Board

## Services performed at satellite laboratory

700 Lairport Street  
El Segundo, CA 90245

Glenn Gaza 310-643-0438

[glenn.gaza@keysight.com](mailto:glenn.gaza@keysight.com)

[www.keysight.com](http://www.keysight.com)

### Acoustics and Vibration

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Accelerometers – Source and Measure	Sinusoidal (2 to 4) Hz 5 Hz to 2 kHz (2 to 10) kHz	2.5% of reading 1.5% of reading 2.5% of reading	Comparison to a reference accelerometer
	Shock (2 to 10) g	2 % of reading	Comparison to a standard shock accelerometer

### Electrical – DC/Low Frequency

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
DC Voltage – Source	0 V 100 mV 1 V 10 V 100 V 1 000 V	54 nV 91 nV 0.32 $\mu$ V 2.5 $\mu$ V 38 $\mu$ V 0.66 mV	Comparison to DC voltage standard characterized by a Keysight 3458A multimeter
DC Voltage – Source	(>0 to 220) mV (0.22 to 2.2) V (2.2 to 11) V (11 to 22) V (22 to 220) V (220 V to 1 100) V	7 $\mu$ V/V + 0.39 $\mu$ V 4.7 $\mu$ V/V + 0.62 $\mu$ V 3.1 $\mu$ V/V + 2.3 $\mu$ V 3.1 $\mu$ V/V + 4.2 $\mu$ V 4.7 $\mu$ V/V + 39 $\mu$ V 6.2 $\mu$ V/V + 0.39 mV	Direct comparison to a DC voltage standard
DC Voltage – Source	(2 to 60) kV	40 $\mu$ V/V	Comparison to a voltage divider
DC Voltage – Measure	(>0 to 0.1) V (0.1 to 1) V (1 to 10) V (10 to 100) V (100 to 1 000) V	4.1 $\mu$ V/V + 0.36 $\mu$ V 3.7 $\mu$ V/V + 0.35 $\mu$ V 3.1 $\mu$ V/V + 0.59 $\mu$ V 5.3 $\mu$ V/V + 36 $\mu$ V 5.3 $\mu$ V/V + 0.12 mV	Direct measurement with a Keysight 3458A multimeter



ANSI National Accreditation Board

Electrical – DC/Low Frequency

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
DC Voltage – Measure (Differential)	(>0 to 0.1) V (0.1 to 1) V (1 to 10) V (10 to 100) V (100 to 1 000) V	0.61 $\mu\text{V/V} + 0.061 \mu\text{V}$ 0.37 $\mu\text{V/V} + 0.12 \mu\text{V}$ 0.061 $\mu\text{V/V} + 0.61 \mu\text{V}$ 0.61 $\mu\text{V/V} + 0.012 \text{ mV}$ 1.8 $\mu\text{V/V} + 0.061 \text{ mV}$	Differential measurement with a Keysight 3458A multimeter
DC Current – Source	0 A 100 $\mu\text{A}$ 1 mA 10 mA 100 mA 1 A	42 pA 0.15 nA 1.5 nA 17 nA 0.47 $\mu\text{A}$ 9.6 $\mu\text{A}$	Comparison to a DC source characterized with a Keysight 3458A multimeter
DC Current – Source	(>0 to 220) $\mu\text{A}$ (0.22 to 2.2) mA (2.2 to 22) mA (22 to 100) mA (100 to 200) mA (0.22 to 1) A (1 to 1.6) A (1.6 to 2.2) A (2.2 to 11) A (11 to 20.5) A	39 $\mu\text{A/A} + 5.4 \text{ nA}$ 31 $\mu\text{A/A} + 6.3 \text{ nA}$ 31 $\mu\text{A/A} + 39 \text{ nA}$ 39 $\mu\text{A/A} + 0.62 \mu\text{A}$ 52 $\mu\text{A/A} - 0.74 \mu\text{A}$ 70 $\mu\text{A/A} + 12 \mu\text{A}$ 110 $\mu\text{A/A} - 21 \mu\text{A}$ 150 $\mu\text{A/A} - 92 \mu\text{A}$ 280 $\mu\text{A/A} + 370 \mu\text{A}$ 0.82 mA/A + 0.89 $\mu\text{A}$	Comparison to a DC current source
DC Current – Source	(10 to 1 025) A	0.2 % of reading	Comparison to DC current source and a current coil
DC Current – Source and Measure	1 $\mu\text{A}$ to 30 mA (30 to 100) mA (100 to 300) mA (300 to 400) mA (500 to 800) mA (800 to 900) mA 900 mA to 15 A (16 to 50) A (50 to 70) A (70 to 100) A (100 to 400) A	4 $\mu\text{A/A}$ 5 $\mu\text{A/A}$ 6 $\mu\text{A/A}$ 13 $\mu\text{A/A}$ 11 $\mu\text{A/A}$ 9 $\mu\text{A/A}$ 8 $\mu\text{A/A}$ 13 $\mu\text{A/A}$ 18 $\mu\text{A/A}$ 24 $\mu\text{A/A}$ 30 $\mu\text{A/A}$	Comparison to DC source, standard resistor and a voltmeter
DC Current – Measure	(0.10 to 1) A (1 to 100) A (100 to 500) A (500 to 1 000) A	73 $\mu\text{A/A} + 1.3 \mu\text{A}$ 74 $\mu\text{A/A} - 0.021 \mu\text{A}$ 58 $\mu\text{A/A} + 180 \mu\text{A}$ 140 $\mu\text{A/A} + 0.42 \text{ mA}$	Comparison to a DC current shunt and a Keysight 3458A multimeter

**Electrical – DC/Low Frequency**

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
DC Current – Measure	(5 to 10) A (10 to 30) A (30 to 36) A (36 to 45) A (45 to 60) A (60 to 90) A (90 to 180) A (180 to 340) A (340 to 510) A (510 to 1 000) A (1 000 to 2 000) A	93 $\mu$ A/A + 0.39 mA 140 $\mu$ A/A 94 $\mu$ A/A + 1.5 mA 92 $\mu$ A/A + 1.9 mA 93 $\mu$ A/A + 2.6 mA 91 $\mu$ A/A + 4 mA 87 $\mu$ A/A + 8.5 mA 200 $\mu$ A/A 180 $\mu$ A/A + 8.8 mA 180 $\mu$ A/A + 18 mA 150 $\mu$ A/A + 26 mA	Comparison to a DC current transducer and a Keysight 3458A multimeter
DC Current – Measure	0 pA (0.1 to 1.15) pA (1 to 115) pA (10 to 115) pA (0.1 to 1.15) nA (1 to 11.5) nA (10 to 115) nA (0.1 to 1.15) $\mu$ A (1 to 11.5) $\mu$ A	0.49 fA 0.83 mA/A + 0.59 fA 0.92 mA/A + 0.38 fA 0.24 mA/A + 1.4 fA 0.24 mA/A + 21 fA 26 $\mu$ A/A + 0.25 pA 51 $\mu$ A/A + 0.54 pA 20 $\mu$ A/A + 1.7 pA 13 $\mu$ A/A + 28 pA	Comparison to a Keysight 3458A multimeter and reference resistors
DC Current – Measure	(0 to 100) nA (0.1 to 1) $\mu$ A (1 to 10) $\mu$ A (10 to 100) $\mu$ A (0.1 to 1) mA (1 to 10) mA (10 to 100) mA (0.1 to 1) A (1 to 3) A	42 $\mu$ A/A + 50 pA 21 $\mu$ A/A + 50 pA 25 $\mu$ A/A + 0.11 nA 25 $\mu$ A/A + 0.85 nA 22 $\mu$ A/A + 6.4 nA 23 $\mu$ A/A + 59 nA 41 $\mu$ A/A + 0.6 $\mu$ A 125 $\mu$ A/A + 12 $\mu$ A 1.4 mA/A + 0.74 mA	Direct measurement with a Keysight multimeter
DC Current – Measure (Differential)	10 $\mu$ A to 100 $\mu$ A 100 $\mu$ A to 1 mA	24 $\mu$ A/A + 0.97 nA 24 $\mu$ A/A + 6.1 nA	Direct measurement with a Keysight 3458A multimeter

**Electrical – DC/Low Frequency**

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
DC Current – Measure (Differential)	1 mA to 10 mA 10 mA to 100 mA 100 mA to 1.0 A 1 A to 10 A 10 A to 30 A 30 A to 50 A 50 A to 100 A 100 A to 300 A 300 A to 500 A 500 A to 1 000 A	0.61 $\mu$ A/A + 6.1 nA 0.061 $\mu$ A/A + 6 nA 0.061 $\mu$ A/A + 61 nA 0.061 $\mu$ A/A + 1 $\mu$ A 0.061 $\mu$ A/A + 6.1 $\mu$ A 0.061 $\mu$ A/A + 12 $\mu$ A 0.37 $\mu$ A/A + 12 $\mu$ A 0.37 $\mu$ A/A + 0.12 mA 0.37 $\mu$ A/A + 0.24 mA 0.61 $\mu$ A/A + 0.61 mA	Comparison to a Keysight 3458A multimeter and a resistive shunt
AC Voltage – Measure	(1 to 80) kV 60 Hz	0.19 % of reading	Comparison to a voltage divider
AC Current – Source	1 kHz 10 $\mu$ A 100 $\mu$ A 1 mA 10 mA 100 mA 1 A	3 nA 2.5 nA 32 nA 330 nA 3.3 $\mu$ A 38 $\mu$ A	Comparison to a multifunction calibrator and a Keysight 3458A multimeter
AC Current - Source	60 Hz 2.5A 5 A	365 $\mu$ A 669 $\mu$ A	Comparison to an AC shunt and a Keysight 3458A multimeter
AC Current – Source (Relative) <sup>1</sup>	100 kHz to 100 MHz Ratio 0.7 to 1.1	0.058	Comparison to an oscilloscope
AC Current - Measure	(45 to 100) Hz 2.5 A, 60 Hz 2.5 A, 500 Hz 5 A, 60 Hz 5 A, 500 Hz 10 A, (60, 500) Hz 20 A, (60, 500) Hz 40 A, (60, 500) Hz	0.6 mA 1.2 mA 1.1 mA 2.4 mA 4.9 mA 9.5 mA 19 mA	Comparison to a resistive shunt and a Keysight 3458A multimeter

**Electrical – DC/Low Frequency**

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Resistance – Source	(0.1 to 0.2) mΩ	7.2 μΩ/Ω	Comparison to Guildline 6675A Bridge, 6623 Extender, L&N Standard Resistors, ESIU SR 1010, SR 1050, Hart 7009 Oil Bath, MI 9300 Air Bath
	(0.2 to 0.3) mΩ	4.3 μΩ/Ω	
	(0.3 to 0.4) mΩ	3.3 μΩ/Ω	
	(0.4 to 1) mΩ	2.9 μΩ/Ω	
	(1 to 2) mΩ	1.4 μΩ/Ω	
	(3 to 5) mΩ	3.4 μΩ/Ω	
	(6 to 9) mΩ	2.4 μΩ/Ω	
	(10 to 20) mΩ	1.5 μΩ/Ω	
	(3 to 5) mΩ	3.4 μΩ/Ω	
	(6 to 9) mΩ	2.4 μΩ/Ω	
	(0.3 to 0.5) Ω	1.4 μΩ/Ω	
	(0.6 to 0.9) Ω	1 μΩ/Ω	
	(1 to 13) Ω	0.17 μΩ/Ω	
	14 Ω to 1 kΩ	0.38 μΩ/Ω	
	(1.1 to 9) kΩ	0.4 μΩ/Ω	
	(11 to 100) kΩ	0.45 μΩ/Ω	
200 kΩ to 1 MΩ	0.84 μΩ/Ω		
(2 to 10) MΩ	1.8 μΩ/Ω		
(11 to 100) MΩ	4.1 μΩ/Ω		
(200 to 900) MΩ	12 μΩ/Ω		
Resistance – Source	0.1 Ω	0.62 μΩ/Ω	Comparison to Guildline 6675Av Bridge, 6623 Extender, L&N Standard Resistors, ESIU SR 1010, SR 1050, Hart 7009 Oil Bath, MI 9300 Air Bath
	0.2 Ω	0.64 μΩ/Ω	
	1 Ω	0.17 μΩ/Ω	
	10 Ω	0.17 μΩ/Ω	
	100 Ω	0.38 μΩ/Ω	
	1 kΩ	0.38 μΩ/Ω	
	10 kΩ	0.25 μΩ/Ω	
	1 GΩ	12 μΩ/Ω	
Resistance – Source	1 Ω	86 μΩ/Ω	Comparison to a multifunction calibrator
	1.9 Ω	85 μΩ/Ω	
	(10, 19) Ω	21 μΩ/Ω	
	(100, 190) Ω	9.3 μΩ/Ω	
	(1, 1.9, 10, 19) kΩ	6.2 μΩ/Ω	
	100 kΩ	7.8 μΩ/Ω	
	190 kΩ	9.3 μΩ/Ω	
	1 MΩ	12 μΩ/Ω	
	1.9 MΩ	16 μΩ/Ω	
	10 MΩ	36 μΩ/Ω	
19 MΩ	43 μΩ/Ω		
100 MΩ	93 μΩ/Ω		

**Electrical – DC/Low Frequency**

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Resistance – Source	(>0 to 11) Ω (11 to 110) Ω (0.11 to 1.1) kΩ (1.1 to 3.3) kΩ (3.3 to 11) kΩ (11 to 110) kΩ 110 kΩ to 1.1 MΩ (1.1 to 3.3) MΩ (3.3 to 11) MΩ (11 to 33) MΩ (33 to 110) MΩ (110 to 330) MΩ (330 to 1 100) MΩ	33 μΩ/Ω + 8.3 mΩ 25 μΩ/Ω + 12.5 mΩ 23 μΩ/Ω + 17 mΩ 23 μΩ/Ω + 170 mΩ 23 μΩ/Ω + 84 mΩ 23 μΩ/Ω + 0.84 Ω 27 μΩ/Ω + 8 Ω 50 μΩ/Ω + 125 Ω 110 μΩ/Ω + 0.2 kΩ 210 μΩ/Ω + 2 kΩ 410 μΩ/Ω + 2.8 kΩ 2.5 mΩ/Ω + 83 kΩ 12 mΩ/Ω + 0.4 MΩ	Comparison to a multiproduct calibrator
Resistance – Source and Measure	0 Ω 10 Ω 100 Ω 1 kΩ 10 kΩ 100 kΩ 1 MΩ 10 MΩ 100 MΩ	7.6 μΩ 13 μΩ 76 μΩ 0.40 mΩ 4.5 mΩ 42 mΩ 0.88 Ω 22 Ω 1.3 kΩ	Comparison to multifunction calibrator and a Keysight 3458A multimeter
Resistance - Measure	(1 to 10) GΩ (10 to 100) GΩ 100 GΩ to 1 TΩ (1 to 10) TΩ (10 to 100) TΩ 100 TΩ to 1 PΩ (1 to 10) PΩ	0.8 mΩ/Ω 1.2 mΩ/Ω 2.3 mΩ/Ω 3.5 mΩ/Ω 5.8 mΩ/Ω 12 mΩ/Ω 0.12 Ω/Ω	Comparison to Guildline 6500A Terohmmeter
Resistance - Measure	(0 to 12) Ω (12 to 100) Ω (0.1 to 1.2) kΩ (1.2 to 12) kΩ (12 to 120) kΩ (0.12 to 1.2) MΩ (1.2 to 12) MΩ (12 to 120) MΩ (0.12 to 1.2) GΩ	20 μΩ/Ω + 79 μΩ 15 μΩ/Ω + 0.79 mΩ 13 μΩ/Ω + 0.79 mΩ 13 μΩ/Ω + 7.8 mΩ 13 μΩ/Ω + 78 mΩ 17 μΩ/Ω + 2.6 Ω 61 μΩ/Ω + 0.12 kΩ 0.58 mΩ/Ω + 3.6 kΩ 5.7 mΩ/Ω + 0.26 MΩ	Comparison to a Keysight 3458A multimeter

**Electrical – DC/Low Frequency**

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Capacitance – Measure	50 Hz to 20 kHz		Comparison to a capacitance bridge
	(1 to 2) pF	4.1 $\mu$ F/F	
	(2 to 4) pF	3.7 $\mu$ F/F	
	(4 to 9) pF	3.6 $\mu$ F/F	
	(10, 20, 30) pF	3.6 $\mu$ F/F	
	(40 to 100) pF	3.5 $\mu$ F/F	
	(300 to 400) pF	3.5 $\mu$ F/F	
	(500 to 600) pF	3.6 $\mu$ F/F	
	(700 to 800) pF	3.5 $\mu$ F/F	
	0.9 pF to 1 nF	3.6 $\mu$ F/F	
	(1 to 4) nF	3.6 $\mu$ F/F	
	(4 to 10) nF	3.7 $\mu$ F/F	
	(10 to 40) nF	3.9 $\mu$ F/F	
	(40 to 100) nF	4.7 $\mu$ F/F	
	(100 to 400) nF	7.4 $\mu$ F/F	
(400 to 1200) nF	15 $\mu$ F/F		
Capacitance – Measure	50 Hz to 20 kHz		Comparison to Standard Capacitors
	1 pF	4.1 $\mu$ F/F	
	2 pF	3.8 $\mu$ F/F	
	0.2 nF	3.6 $\mu$ F/F	
Capacitance – Source	(0.19 to 3.29) nF	3.1 mF/F + 7.7 pF	Comparison to a multiproduct calibrator
	(3.3 to 10.99) nF	1.4 mF/F + 8.2 pF	
	(11 to 109.99) nF	1.4 mF/F + 80 pF	
	(110 to 329.99) nF	1.5 mF/F + 0.24 nF	
	(0.33 to 1.099) $\mu$ F	1.4 mF/F + 0.82 nF	
	(1.1 to 3.299) $\mu$ F	1.5 mF/F + 2.4 nF	
	(3.3 to 10.99) $\mu$ F	1.4 mF/F + 8.1 nF	
	(11 to 32.99) $\mu$ F	2.4 mF/F + 24 nF	
	(33 to 109.99) $\mu$ F	2.6 mF/F + 83 nF	
	(110 to 329.99) $\mu$ F	2.7 mF/F + 0.24 $\mu$ F	
	(0.33 to 1.099) mF	2.6 mF/F + 0.82 $\mu$ F	
	(1.1 to 3.299) mF	2.7 mF/F + 2.4 $\mu$ F	
	(3.3 to 10.00) mF	3.3 mF/F + 5.2 $\mu$ F	
	(11 to 32.99) mF	5.5 mF/F + 24 $\mu$ F	
(33 to 110) mF	7.9 mF/F + 79 $\mu$ F		

**Electrical – DC/Low Frequency**

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Capacitance – Source	10 pF		Comparison to Standard Capacitors
	50 Hz	3.4 $\mu$ F/F	
	0.1 kHz	1.6 $\mu$ F/F	
	0.4 kHz	0.48 $\mu$ F/F	
	0.8 kHz	0.35 $\mu$ F/F	
	1 kHz	0.33 $\mu$ F/F	
	2 kHz	0.32 $\mu$ F/F	
	6 kHz	0.55 $\mu$ F/F	
	8 kHz	0.75 $\mu$ F/F	
	10 kHz	1.1 $\mu$ F/F	
	16 kHz	2.3 $\mu$ F/F	
20 kHz	3.5 $\mu$ F/F		
Capacitance – Source	100 pF		Comparison to Standard Capacitors
	50 Hz	1.9 $\mu$ F/F	
	0.1 kHz	1 $\mu$ F/F	
	0.4 kHz	0.54 $\mu$ F/F	
	0.8 kHz	0.46 $\mu$ F/F	
	1 kHz	0.29 $\mu$ F/F	
	2 kHz	0.28 $\mu$ F/F	
	6 kHz	0.45 $\mu$ F/F	
	8 kHz	0.81 $\mu$ F/F	
	10 kHz	0.94 $\mu$ F/F	
	16 kHz	2.1 $\mu$ F/F	
20 kHz	2.7 $\mu$ F/F		
Capacitance – Source	1 000 pF		Comparison to Standard Capacitors
	0.1 kHz	3.7 $\mu$ F/F	
	0.4 kHz	2.7 $\mu$ F/F	
	1 kHz	2.3 $\mu$ F/F	

**Electrical – DC/Low Frequency**

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Capacitance – Source	1 pF		Comparison to Standard Capacitors
	1 kHz	30 $\mu$ F/F	
	10 kHz	33 $\mu$ F/F	
	50 kHz	55 $\mu$ F/F	
	100 kHz	83 $\mu$ F/F	
	500 kHz	0.35 mF/F	
	1 MHz	0.71 mF/F	
	2 MHz	1.6 mF/F	
	3 MHz	2.8 mF/F	
	4 MHz	3.8 mF/F	
	5 MHz	5.1 mF/F	
	6 MHz	6.6 mF/F	
	7 MHz	8.2 mF/F	
8 MHz	10 mF/F		
9 MHz	12 mF/F		
10 MHz	14 mF/F		
Capacitance – Source	10 pF		Comparison to Standard Capacitors
	1 kHz	29 $\mu$ F/F	
	10 kHz	33 $\mu$ F/F	
	50 kHz	33 $\mu$ F/F	
	100 kHz	33 $\mu$ F/F	
	500 kHz	33 $\mu$ F/F	
	1 MHz	33 $\mu$ F/F	
	2 MHz	54 $\mu$ F/F	
	3 MHz	0.1 mF/F	
	4 MHz	0.17 mF/F	
	5 MHz	0.27 mF/F	
	6 MHz	0.39 mF/F	
	7 MHz	0.53 mF/F	
8 MHz	0.7 mF/F		
9 MHz	0.9 mF/F		
10 MHz	1.1 mF/F		

**Electrical – DC/Low Frequency**

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Inductance – Source and Measure	100 $\mu$ H		Comparison to LCR Meter, Standard Inductors
	100 Hz	0.15 mH/H	
	1 kHz	80 $\mu$ H/H	
	10 kHz	0.15 mH/H	
	1 mH		
	100 Hz	0.1 mH/H	
	1 kHz	70 $\mu$ H/H	
	10 kHz	0.15 mH/H	
	10 mH		
	1 kHz	70 $\mu$ H/H	
	10 kHz	0.13 mH/H	
	100 mH		
	100 Hz	90 $\mu$ H/H	
	1 kHz	70 $\mu$ H/H	
	10 Hz	0.2 mH/H	
1 H			Comparison to Clark-Hess 5500-2 Phase Standard
(100, 400) Hz	80 $\mu$ H/H		
1 kHz	70 $\mu$ H/H		
10 H			
(100, 400) Hz	90 $\mu$ H/H		
1 kHz	80 $\mu$ H/H		
(0 to 360) $^{\circ}$			
@ 5V Equal Input	0.005 $^{\circ}$		
1 Hz to 6.25 kHz	0.012 $^{\circ}$		
(6.25 to 50) kHz	0.047 $^{\circ}$		
(50 to 200) kHz			
@50 mV to 100V	0.006 $^{\circ}$		
1 Hz to 1 kHz	0.012 $^{\circ}$		
(1 to 6.25) kHz	0.018 $^{\circ}$		
(6.25 to 50) kHz	0.047 $^{\circ}$		
(50 to 200) kHz			
@100V to 120V	0.01 $^{\circ}$		
1 Hz to 1 kHz	0.02 $^{\circ}$		
(1 to 6.25) kHz	0.035 $^{\circ}$		
(6.25 to 50) kHz	0.093 $^{\circ}$		
(50 to 200) kHz			

**Electrical – DC/Low Frequency**

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Phase Angle – Measure	(0 to 360)°		Comparison to Clark-Hess 6000A Phase Meter
	10 mV to 350V		
	(5 to 10) Hz	0.23°	
	10 Hz to 50 kHz	0.06°	
	(50 to 57) kHz	0.12°	
	(57 to 66) kHz	0.13°	
	(66 to 75) kHz	0.14°	
	(75 to 83) kHz	0.15°	
	(83 to 92) kHz	0.16°	
	(92 to 100) kHz	0.17°	
	101 kHz	0.57°	
	110 kHz	0.62°	
	115 kHz	0.64°	
	120 kHz	0.67°	
	125 kHz	0.69°	
	130 kHz	0.72°	
	135 kHz	0.74°	
	140 kHz	0.77°	
145 kHz	0.79°		
150 kHz	0.82°		
200 kHz	1.1°		
250 kHz	1.4°		
300 kHz	1.6°		
350 kHz	1.9°		
400 kHz	2.1°		
450 kHz	2.4°		
500 kHz	2.6°		
Ratio Transformer	400 Hz, 1 kHz	0.000 051 % of Input	Comparison to Gertsch 1011 Ratio Standard

**Electrical – DC/Low Frequency**

El Segundo, CA

Parameter/Equipment	AC Voltage - Source							
Reference Standard, Method, and/or Equipment	Comparison to a characterized AC voltage source							
Expanded Uncertainty of Measurement (+/-)								
Range	10 mV	100 mV	1 V	3 V	10 V	100 V	700 V	1000 V
10 Hz	0.69 μV	1.7 μV	-	-	76 μV	-	-	-



ANSI National Accreditation Board

Electrical – DC/Low Frequency

El Segundo, CA

Parameter/Equipment	AC Voltage - Source							
Reference Standard, Method, and/or Equipment	Comparison to a characterized AC voltage source							
Expanded Uncertainty of Measurement (+/-)								
Range	10 mV	100 mV	1 V	3 V	10 V	100 V	700 V	1000 V
20 Hz	0.51 $\mu$ V	1.8 $\mu$ V	-	-	45 $\mu$ V	-	-	-
40 Hz	-	-	-	-	35 $\mu$ V	-	-	-
200 Hz	-	-	-	-	24 $\mu$ V	-	-	-
500 Hz	-	-	-	-	25 $\mu$ V	-	-	-
1 kHz	70 nV	0.36 $\mu$ V	2.6 $\mu$ V	-	26 $\mu$ V	0.42 mV	6.5 mV	16 mV
10 kHz	-	-	-	-	26 $\mu$ V	-	7 mV	11 mV
20 kHz	76 nV	0.31 $\mu$ V	2.8 $\mu$ V	-	25 $\mu$ V	0.35 mV	-	22 mV
50 kHz	-	-	3.7 $\mu$ V	-	36 $\mu$ V	0.67 mV	-	-
100 kHz	62 nV	0.34 $\mu$ V	4.6 $\mu$ V	13 $\mu$ V	44 $\mu$ V	0.8 mV	-	-
300 kHz	0.17 $\mu$ V	0.7 $\mu$ V	8 $\mu$ V	-	73 $\mu$ V	-	-	-
500 kHz	-	-	11 $\mu$ V	-	0.11 mV	-	-	-
1 MHz	1.2 $\mu$ V	2.7 $\mu$ V	20 $\mu$ V	-	0.19 mV	-	-	-
2 MHz	-	-	-	2.1 mV	-	-	-	-
4 MHz	10 $\mu$ V	0.1 mV	1 mV	3.2 mV	-	-	-	-
8 MHz	-	0.16 mV	1.6 mV	4.8 mV	-	-	-	-
10 MHz	-	0.18 mV	1.8 mV	5.5 mV	-	-	-	-

Electrical – DC/Low Frequency

El Segundo, CA

Parameter/Equipment	AC Voltage - Source								
Reference Standard, Method, and/or Equipment	Comparison to an AC voltage source								
Expanded Uncertainty of Measurement (+/-)									
Range	(>0 to 2.2) mV	(2.2 to 22) mV	(22 to 220) mV	(0.22 to 2.2) V	(2.2 to 22) V	(22 to 220) V	(220 to 250) V	(220 to 100) V	(220 to 750) V
(10 to 15) Hz	230 $\mu$ V/V + 3.9 $\mu$ V	230 $\mu$ V/V + 3.9 $\mu$ V	230 $\mu$ V/V + 12 $\mu$ V	230 $\mu$ V/V + 39 $\mu$ V	230 $\mu$ V/V + 390 $\mu$ V	230 $\mu$ V/V + 3.9 mV	-	-	-
(15 to 20) Hz	230 $\mu$ V/V + 3.9 $\mu$ V	230 $\mu$ V/V + 3.9 $\mu$ V	230 $\mu$ V/V + 12 $\mu$ V	230 $\mu$ V/V + 39 $\mu$ V	230 $\mu$ V/V + 390 $\mu$ V	230 $\mu$ V/V + 3.9 mV	280 $\mu$ V/V + 16 mV	-	-
(20 to 40) Hz	89 $\mu$ V/V + 3.9 $\mu$ V	89 $\mu$ V/V + 3.9 $\mu$ V	89 $\mu$ V/V + 6.2 $\mu$ V	85 $\mu$ V/V + 16 $\mu$ V	85 $\mu$ V/V + 160 $\mu$ V	85 $\mu$ V/V + 1.6 mV	280 $\mu$ V/V + 16 mV	-	-
(40 to 50) Hz	77 $\mu$ V/V + 3.9 $\mu$ V	77 $\mu$ V/V + 3.9 $\mu$ V	54 $\mu$ V/V + 6.2 $\mu$ V	37 $\mu$ V/V + 7.8 $\mu$ V	37 $\mu$ V/V + 54 $\mu$ V	50 $\mu$ V/V + 0.54 mV	-	70 $\mu$ V/V + 3.1 mV	-
50 Hz to 1 kHz	77 $\mu$ V/V + 3.9 $\mu$ V	77 $\mu$ V/V + 3.9 $\mu$ V	54 $\mu$ V/V + 6.2 $\mu$ V	37 $\mu$ V/V + 7.8 $\mu$ V	37 $\mu$ V/V + 54 $\mu$ V	50 $\mu$ V/V + 0.54 mV	-	66 $\mu$ V/V + 3.1 mV	-
(1 to 20) kHz	77 $\mu$ V/V + 3.9 $\mu$ V	77 $\mu$ V/V + 3.9 $\mu$ V	54 $\mu$ V/V + 6.2 $\mu$ V	37 $\mu$ V/V + 7.8 $\mu$ V	37 $\mu$ V/V + 54 $\mu$ V	50 $\mu$ V/V + 0.54 mV	-	130 $\mu$ V/V + 4.7 mV	-





ANSI National Accreditation Board

Electrical – DC/Low Frequency

El Segundo, CA

Parameter/Equipment	AC Voltage - Source								
Reference Standard, Method, and/or Equipment	Comparison to an AC voltage source								
Expanded Uncertainty of Measurement (+/-)									
Range	(>0 to 2.2) mV	(2.2 to 22) mV	(22 to 220) mV	(0.22 to 2.2) V	(2.2 to 22) V	(22 to 220) V	(220 to 250) V	(220 to 100) V	(220 to 750) V
(20 to 30) kHz	190 μV/V + 3.9 μV	190 μV/V + 3.9 μV	120 μV/V + 6.2 μV	62 μV/V + 9.3 μV	62 μV/V + 93 μV	78 μV/V + 0.93 mV	-	470 μV/V + 8.5 mV	-
(30 to 50) kHz	190 μV/V + 3.9 μV	190 μV/V + 3.9 μV	120 μV/V + 6.2 μV	62 μV/V + 9.3 μV	62 μV/V + 93 μV	78 μV/V + 0.93 mV	-	-	470 μV/V + 8.5 mV
(50 to 100) kHz	460 μV/V + 4.7 μV	470 μV/V + 4.7 μV	310 μV/V + 16 μV	78 μV/V + 31 μV	78 μV/V + 190 μV	140 μV/V + 2.3 mV	-	-	1.8 mV/V + 35 mV
Range	(>0 to 2.2) mV	(2.2 to 22) mV	(22 to 220) mV	(0.22 to 2.2) V	(2.2 to 22) V	(22 to 220) V	(220 to 250) V	(220 to 100) V	(220 to 750) V
(100 to 300) kHz	1 mV/V + 9.3 μV	1 mV/V + 9.3 μV	620 μV/V + 19 μV	310 μV/V + 78 μV	230 μV/V + 620 μV	850 μV/V + 16 mV	-	-	-
(300 to 500) kHz	1.3 mV/V + 19 μV	1.3 mV/V + 19 μV	1.3 mV/V + 23 μV	930 μV/V + 190 μV	930 μV/V + 1.9 mV	4.2 mV/V + 39 mV	-	-	-
500 kHz to 1 MHz	2.6 mV/V + 19 μV	2.6 mV/V + 19 μV	2.6 mV/V + 47 μV	1.6 mV/V + 310 μV	1.4 mV/V + 3.1 mV	7.8 mV/V + 78 mV	-	-	-

Electrical - DC/Low Frequency

El Segundo, CA

Parameter/Equipment	AC Voltage - Measure								
Reference Standard, Method, and/or Equipment	Comparison to a Comparison to a Thermal Transfer Standard								
Expanded Uncertainty of Measurement (+/-)									
Range	1 V	2 V	6 V	10 V	20 V	60 V	200 V	600 V	1000 V
10 Hz	14 μV/V	13 μV/V	12 μV/V	16 μV/V	13 μV/V	14 μV/V	23 μV/V	21 μV/V	17 μV/V
20 Hz	9 μV/V	7 μV/V	7 μV/V	9 μV/V	8 μV/V	10 μV/V	13 μV/V	12 μV/V	12 μV/V
40 Hz	9 μV/V	7 μV/V	7 μV/V	8 μV/V	7 μV/V	9 μV/V	11 μV/V	12 μV/V	11 μV/V
100 Hz	7 μV/V	7 μV/V	7 μV/V	8 μV/V	7 μV/V	9 μV/V	10 μV/V	10 μV/V	11 μV/V
1 kHz	11 μV/V	7 μV/V	8 μV/V	9 μV/V	8 μV/V	9 μV/V	10 μV/V	10 μV/V	12 μV/V
10 kHz	12 μV/V	7 μV/V	8 μV/V	9 μV/V	8 μV/V	9 μV/V	11 μV/V	10 μV/V	12 μV/V
20 kHz	13 μV/V	7 μV/V	8 μV/V	10 μV/V	9 μV/V	10 μV/V	10 μV/V	10 μV/V	12 μV/V
50 kHz	9 μV/V	8 μV/V	8 μV/V	11 μV/V	10 μV/V	11 μV/V	13 μV/V	11 μV/V	13 μV/V
100 kHz	8 μV/V	8 μV/V	9 μV/V	11 μV/V	10 μV/V	14 μV/V	15 μV/V	15 μV/V	24 μV/V
300 kHz	12 μV/V	13 μV/V	11 μV/V	12 μV/V	11 μV/V	19 μV/V	-	-	-
500 kHz	15 μV/V	21 μV/V	16 μV/V	18 μV/V	15 μV/V	-	-	-	-
800 kHz	20 μV/V	27 μV/V	19 μV/V	20 μV/V	19 μV/V	-	-	-	-
1 MHz	27 μV/V	31 μV/V	25 μV/V	26 μV/V	25 μV/V	-	-	-	-



**Electrical – DC/Low Frequency**

El Segundo, CA

Parameter/Equipment	AC Voltage - Measure					
Reference Standard, Method, and/or Equipment	Comparison to a Keysight 3458A multimeter					
Expanded Uncertainty of Measurement (+/-)						
Range	(>0 to 10 mV)	(10 to 120) mV	(0.12 to 1.2) V	(1.2 to 12) V	(12 to 120) V	(120 to 700) V
(1 to 40) Hz	0.35 mV/V + 3.4 $\mu$ V	83 $\mu$ V/V + 4.6 $\mu$ V	83 $\mu$ V/V + 46 $\mu$ V	83 $\mu$ V/V + 0.46 mV	0.23 mV/V + 4.6 mV	0.46 mV/V + 46 mV
40 Hz to 1 kHz	0.23 mV/V + 1.3 $\mu$ V	83 $\mu$ V/V + 2.3 $\mu$ V	83 $\mu$ V/V + 23 $\mu$ V	83 $\mu$ V/V + 0.23 mV	0.23 mV/V + 2.3 mV	0.46 mV/V + 23 mV
(1 to 20) kHz	0.34 mV/V + 1.3 $\mu$ V	0.16 mV/V + 2.3 $\mu$ V	0.16 mV/V + 23 $\mu$ V	0.16 mV/V + 0.23 mV	0.23 mV/V + 2.3 mV	0.7 mV/V + 23 mV
(20 to 50) kHz	1.1 mV/V + 1.3 $\mu$ V	0.34 mV/V + 2.3 $\mu$ V	0.34 mV/V + 23 $\mu$ V	0.34 mV/V + 0.23 mV	0.4 mV/V + 2.3 mV	1.4 mV/V + 23 mV
(50 to 100) kHz	5.7 mV/V + 1.2 $\mu$ V	0.92 mV/V + 2.3 $\mu$ V	0.92 mV/V + 23 $\mu$ V	0.92 mV/V + 0.23 mV	1.4 mV/V + 2.3 mV	3.5 mV/V + 23 mV
(100 to 300) kHz	46 mV/V + 2.3 $\mu$ V	3.4 mV/V + 12 $\mu$ V	3.4 mV/V + 0.11 mV	3.4 mV/V + 1.2 mV	4.6 mV/V + 11 mV	-
300 kHz to 1 MHz	14 mV/V + 5.8 $\mu$ V	11 mV/V + 12 $\mu$ V	11 mV/V + 0.12 mV	11 mV/V + 1.2 mV	17 mV/V + 11 mV	-
(1 to 2) MHz	81 mV/V + 8.1 $\mu$ V	17 mV/V + 12 $\mu$ V	17 mV/V + 0.12 mV	17 mV/V + 1.2 mV	-	-
(2 to 4) MHz	82 mV/V + 8.1 $\mu$ V	46 mV/V + 81 $\mu$ V	46 mV/V + 0.81 mV	46 mV/V + 8.1 mV	-	-
(4 to 8) MHz	230 mV/V + 9.2 $\mu$ V	46 mV/V + 92 $\mu$ V	46 mV/V + 0.92 mV	46 mV/V + 9.2 mV	-	-
(8 to 10) MHz	-	170 mV/V + 120 $\mu$ V	170 mV/V + 1.2 mV	170 mV/V + 12 mV	-	-

**Electrical – DC/Low Frequency**

El Segundo, CA

Parameter/Equipment	AC Current - Source									
Reference Standard, Method, and/or Equipment	Comparison to an AC source									
Expanded Uncertainty of Measurement (+/-)										
Range	(10 to 20) Hz	(20 to 30) Hz	(30 to 40) Hz	(40 to 45) Hz	(45 to 100) Hz	(0.1 to 1) kHz	(1 to 5) kHz	(5 to 10) kHz	(10 to 30) kHz	
(>0 to 220) $\mu$ A	230 $\mu$ A/A + 16 nA	160 $\mu$ A/A + 9.3 nA	160 $\mu$ A/A + 9.3 nA	93 $\mu$ A/A + 7.8 nA	93 $\mu$ A/A + 7.8 nA	93 $\mu$ A/A + 7.8 nA	270 $\mu$ A/A + 12 nA	1 mA/A + 62 nA	13 mA/A + 0.33 $\mu$ A	
(220 to 330) $\mu$ A	230 $\mu$ A/A + 39 nA	160 $\mu$ A/A + 31 nA	160 $\mu$ A/A + 31 nA	93 $\mu$ A/A + 31 nA	93 $\mu$ A/A + 31 nA	93 $\mu$ A/A + 31 nA	190 $\mu$ A/A + 100 nA	1 mA/A + 620 nA	13 mA/A + 0.33 $\mu$ A	
(0.33 to 2.2) mA	230 $\mu$ A/A + 39 nA	160 $\mu$ A/A + 31 nA	160 $\mu$ A/A + 31 nA	93 $\mu$ A/A + 31 nA	93 $\mu$ A/A + 31 nA	93 $\mu$ A/A + 31 nA	190 $\mu$ A/A + 100 nA	1 mA/A + 620 nA	8.2 mA/A + 0.49 $\mu$ A	
(2.2 to 3.3) mA	230 $\mu$ A/A + 390 nA	160 $\mu$ A/A + 310 nA	160 $\mu$ A/A + 310 nA	93 $\mu$ A/A + 310 nA	93 $\mu$ A/A + 310 nA	93 $\mu$ A/A + 310 nA	190 $\mu$ A/A + 540 nA	1 mA/A + 4.7 $\mu$ A	8.2 mA/A + 0.49 $\mu$ A	

**Electrical – DC/Low Frequency**

El Segundo, CA

Parameter/Equipment	AC Current - Source								
Reference Standard, Method, and/or Equipment	Comparison to an AC source								
Expanded Uncertainty of Measurement (+/-)									
Range	(10 to 20) Hz	(20 to 30) Hz	(30 to 40) Hz	(40 to 45) Hz	(45 to 100) Hz	(0.1 to 1) kHz	(1 to 5) kHz	(5 to 10) kHz	(10 to 30) kHz
(3.3 to 22) mA	230 μA/A + 390 nA	160 μA/A + 310 nA	160 μA/A + 310 nA	93 μA/A + 310 nA	93 μA/A + 310 nA	93 μA/A + 310 nA	190 μA/A + 540 nA	1 mA/A + 4.7 μA	3.3 mA/A + 3.3 μA
(22 to 33) mA	230 μA/A + 3.9 μA	160 μA/A + 3.1 μA	160 μA/A + 3.1 μA	93 μA/A + 2.3 μA	93 μA/A + 2.3 μA	93 μA/A + 2.3 μA	190 μA/A + 3.1 μA	1 mA/A + 9.3 μA	3.3 mA/A + 3.3 μA
(33 to 220) mA	230 μA/A + 3.9 μA	160 μA/A + 3.1 μA	160 μA/A + 3.1 μA	93 μA/A + 2.3 μA	93 μA/A + 2.3 μA	93 μA/A + 2.3 μA	190 μA/A + 3.1 μA	1 mA/A + 9.3 μA	3.3 mA/A + 0.16 mA
(220 to 330) mA	1.5 mA/A + 16 μA	230 μA/A + 31 μA	230 μA/A + 31 μA	230 μA/A + 31 μA	230 μA/A + 31 μA	230 μA/A + 31 μA	390 μA/A + 78 μA	6.2 mA/A + 160 μA	3.3 mA/A + 0.16 mA
(0.33 to 2.2) A	1.5 mA/A + 82 μA	230 μA/A + 31 μA	230 μA/A + 31 μA	230 μA/A + 31 μA	230 μA/A + 31 μA	230 μA/A + 31 μA	390 μA/A + 78 μA	6.2 mA/A + 160 μA	-
(2.2 to 3) A	1.5 mA/A + 82 μA	1.5 mA/A + 82 μA	1.5 mA/A + 82 μA	360 μA/A + 130 μA	360 μA/A + 130 μA	360 μA/A + 130 μA	740 μA/A + 290 μA	2.8 mA/A + 580 μA	-
(3 to 11) A	-	-	-	360 μA/A + 130 μA	360 μA/A + 130 μA	360 μA/A + 130 μA	740 μA/A + 290 μA	2.8 mA/A + 580 μA	-
(11 to 20.5) A	-	-	-	-	0.98 mA/A + 4.1 mA	1.2 mA/A + 4.1 mA	25 mA/A + 4.1 mA	-	-

**Electrical - DC/Low Frequency**

El Segundo, CA

Parameter/Equipment	AC Current - Source and Measure						
Reference Standard, Method, and/or Equipment	Comparison to AC shunts and a Thermal Transfer Standard						
Expanded Uncertainty of Measurement (+/-)							
Range	20 Hz	400 Hz	1 kHz	5 kHz	20 kHz	50 kHz	
10 mA	31 μA/A	18 μA/A	18 μA/A	18 μA/A	18 μA/A	29 μA/A	
20 mA	31 μA/A	18 μA/A	18 μA/A	18 μA/A	-	-	
50 mA	31 μA/A	18 μA/A	18 μA/A	18 μA/A	-	-	
100 mA	32 μA/A	21 μA/A	21 μA/A	21 μA/A	21 μA/A	41 μA/A	
200 mA	34 μA/A	22 μA/A	22 μA/A	22 μA/A	-	-	
500 mA	36 μA/A	23 μA/A	23 μA/A	23 μA/A	-	-	
1 A	38 μA/A	25 μA/A	25 μA/A	25 μA/A	-	-	
2 A	25 μA/A	55 μA/A	42 μA/A	27 μA/A	27 μA/A	27 μA/A	

**Electrical – DC/Low Frequency**

El Segundo, CA

<b>Parameter/Equipment</b>	AC Current - Measure			
<b>Reference Standard, Method, and/or Equipment</b>	Comparison to a Keysight 3458A multimeter			
<b>Expanded Uncertainty of Measurement (+/-)</b>				
<b>Range</b>	(10 to 20) Hz	(20 to 45) Hz	(45 to 100) Hz	(0.1 to 5) kHz
(>0 to 120) $\mu$ A	4.6 mA/A + 34 nA	1.7 mA/A + 34 nA	0.69 mA/A + 34 nA	0.69 mA/A + 34 nA
(0.1 to 1.2) mA	4.6 mA/A + 0.23 $\mu$ A	1.7 mA/A + 0.23 $\mu$ A	0.69 mA/A + 0.23 $\mu$ A	0.35 mA/A + 0.23 $\mu$ A
(1 to 12) mA	4.6 mA/A + 2.3 $\mu$ A	1.7 mA/A + 2.3 $\mu$ A	0.69 mA/A + 2.3 $\mu$ A	0.35 mA/A + 2.3 $\mu$ A
(10 to 120) mA	4.6 mA/A + 23 $\mu$ A	1.7 mA/A + 23 $\mu$ A	0.69 mA/A + 23 $\mu$ A	0.35 mA/A + 23 $\mu$ A
(0.12 to 1.05) A	4.6 mA/A + 0.23 mA	1.8 mA/A + 0.23 mA	0.93 mA/A + 0.23 mA	1.1 mA/A + 0.23 mA

**Electrical – DC/Low Frequency**

El Segundo, CA

<b>Parameter/Equipment</b>	AC Current - Measure							
<b>Reference Standard, Method, and/or Equipment</b>	Comparison to an AC source and a current coil							
<b>Expanded Uncertainty of Measurement (+/-)</b>								
(% indicates % of reading where not specified)								
<b>Range</b>	(10 to 20) Hz	(20 to 45) Hz	(45 to 65) Hz	(45 to 100) Hz	45 Hz to 1 kHz	(65 to 400) Hz	(0.1 to 1) kHz	(1 to 5) kHz
(0.1 to 1) mA	0.13% + 0.43 $\mu$ A	0.078% + 0.47 $\mu$ A	-	-	0.058% + 0.5 $\mu$ A	-	-	0.13% + 0.53 $\mu$ A
(1 to 3) mA	0.15% + 0.25 $\mu$ A	0.095% + 0.35 $\mu$ A	-	-	0.075% + 0.35 $\mu$ A	-	-	0.15% + 0.35 $\mu$ A
(3 to 10) mA	0.11% + 5 $\mu$ A	0.063% + 4.4 $\mu$ A	-	-	0.02% + 5.3 $\mu$ A	-	-	0.050% + 5 $\mu$ A
(10 to 30) mA	0.14% + 3 $\mu$ A	0.063% + 4.4 $\mu$ A	-	-	0.02% + 5.3 $\mu$ A	-	-	0.050% + 5 $\mu$ A
(30 to 300) mA	0.12% + 48 $\mu$ A	0.063% + 44 $\mu$ A	-	-	0.02% + 54 $\mu$ A	-	-	0.077% + 58 $\mu$ A
(0.3 to 1) A	0.15% + 86 $\mu$ A	0.12% + 0.4 mA	-	-	0.02% + 0.52 mA	-	-	0.46% + 1 mA
(1 to 2.5) A	0.67% - 0.5 mA	0.46% - 0.5 mA	-	0.1%	-	-	0.14%	0.56% + 0.75 mA
(2.5 to 3) A	-	-	-	0.1%	-	-	0.14%	2.3% + 5 mA
(3 to 10) A	-	-	-	0.034% + 5.1 mA	-	-	0.058% + 5.2 mA	2.3% + 5 mA
(10 to 20) A	-	-	-	0.15% - 6.8 mA	-	-	0.18% - 7 mA	2.3% + 5 mA
(20 to 30)A	-	-	0.24% + 23 mA	-	-	0.58% + 34 mA	-	-
(30 to 150) A	-	-	0.21% + 44 mA	-	-	0.63% + 25 mA	-	-

**Electrical – DC/Low Frequency**

El Segundo, CA

Parameter/Equipment	AC Current - Measure							
Reference Standard, Method, and/or Equipment	Comparison to an AC source and a current coil							
Expanded Uncertainty of Measurement (+/-) (% indicates % of reading where not specified)								
Range	(10 to 20) Hz	(20 to 45) Hz	(45 to 65) Hz	(45 to 100) Hz	45 Hz to 1 kHz	(65 to 400) Hz	(0.1 to 1) kHz	(1 to 5) kHz
(150 to 300) A	-	-	0.23% + 94 mA	-	-	0.64% + 71 mA	-	-
(300 to 1 020) A	-	-	0.25% + 0.19 A	-	-	0.64% + 60 mA	-	-

**Electrical – RF/Microwave**

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Attenuation – Measure Number of attenuation segments 1 or any configuration of multiple segments with attenuation totaling from 1 dB up to and including 40 dB	Type-N, 3.5 mm, 2.4 mm (1 to 40) dB (0.3 to 500) MHz (0.5 to 2) GHz (2 to 18) GHz (18 to 40) GHz (40 to 50) GHz	0.003 4 dB 0.004 7 dB ((0.011 % of reading * f) + 0.004 9) dB 0.008 9 dB 0.012 dB	Comparison to a Keysight network analyzer
Attenuation – Measure Number of attenuation segments 2	Type-N: (50 to 80) dB 3.5 mm: 50, 60 dB 2.4 mm: 50 dB 300 kHz to 8 GHz (8 to 18) GHz (8 to 40) GHz (40 to 50) GHz	0.025 dB 0.029 dB 0.034 dB 0.037 dB	Comparison to a Keysight network analyzer
Attenuation – Measure Number of attenuation segments 3	Type-N: (70 to 100) dB 3.5 mm: 70 dB or 80 dB 300 kHz to 18 GHz (18 to 20) GHz (20 to 40) GHz (40 to 50) GHz	0.048 dB 0.056 dB 0.059 dB 0.065 dB	Comparison to a Keysight network analyzer

**Electrical – RF/Microwave**

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Attenuation – Measure Number of attenuation segments 4	Type-N: 110, 120 dB 3.5 mm: 90 dB 2.4 mm: 65 or 90 dB 300 kHz to 18 GHz (18 to 20) GHz (20 to 40) GHz (40 to 50) GHz	0.072 dB 0.08 dB 0.084 dB 0.094 dB	Comparison to a Keysight network analyzer
RF Power - Measure Power Meter Reference	1 mW, 50 MHz	0.23 % of reading	Comparison to a power meter
RF Power - Measure DC VSWR <sup>1</sup>	1:1 to 2:1	0.000 32	Comparison to a Keysight 3458A multimeter
RF Power - Measure Calibration Factors <sup>1</sup>	(0 to 105) % DC to 9 kHz	0.0039	Comparison to a Keysight 3458A multimeter
RF Power - Measure Calibration Factors <sup>1</sup>	(0.5 to 1.5) 9 kHz to 30 kHz 30 kHz to 50 MHz (50 to 100) MHz (0.1 to 6) GHz (6 to 7) GHz (7 to 8) GHz (8 to 18 GHz) (18 to 26) GHz (26 to 31) GHz (31 to 37 GHz) (37 to 38) GHz (38 to 40) GHz (40 to 46) GHz (46 to 50) GHz (50 to 67) GHz (67 to 75) GHz (75 to 100) GHz (100 to 106) GHz (106 to 108) GHz (108 to 110) GHz (110 to 114) GHz (114 to 120) GHz	0.003 1 0.002 9 0.002 1 0.002 9 0.003 1 0.003 2 0.003 8 0.008 1 0.008 6 0.008 4 0.009 3 0.008 3 0.014 0.013 0.02 0.041 0.044 0.043 0.045 0.051 0.054 0.057	Comparison to a power sensor



ANSI National Accreditation Board

Electrical – RF/Microwave

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
RF Power - Measure (Relative)	(Ref -30 to 11 dBm)		Comparison to power sensors
	900 Hz to 9 kHz		
	(-40 to -35) dB	0.14 dB	
	(-35 to -30) dB	0.051 dB	
	(-30 to -3) dB	0.026 dB	
	(-3 to 3) dB	0.006 1 dB	
	(3 to 10) dB	0.014 dB	
	(10 to 30) dB	0.023 dB	
	9 kHz to 50 GHz		
	(-130 to -110) dB	0.17 dB	
	(-110 to -100) dB		
	(9 to 100) kHz	0.064 dB	
	100 kHz to 3.6 GHz	0.05 dB	
	(3.6 to 30) GHz	0.07 dB	
	(30 to 50) GHz	0.074 dB	
	(-100 to -90) dB	0.044 dB	
	(-90 to -70) dB	0.034 dB	
	(-70 to -50) dB	0.029 dB	
	(-50 to -30) dB	0.018 dB	
	(-30 to -10) dB	0.009 2 dB	
	(-10 to -5) dB	0.006 5 dB	
	(-5 to 5) dB	0.002 2 dB	
	(5 to 10) dB	0.006 5 dB	
	(10 to 20) dB	0.092 dB	
	(20 to 30) dB	0.026 dB	
	(50 to 67) GHz		
	(-130 to -120) dB	0.22 dB	
	(-120 to -80) dB	0.17 dB	
	(-80 to -70) dB	0.21 dB	
	(-70 to -60) dB	0.05 dB	
	(-60 to -50) dB	0.033 dB	
	(-50 to -40) dB	0.025 dB	
(-40 to -35) dB	0.021 dB		
(-35 to -30) dB	0.019 dB		
(-30 to -3) dB	0.005 6 dB		
(-3 to 3) dB	0.002 2 dB		
(3 to 10) dB	0.014 dB		
(10 to 30) dB	0.023 dB		

**Electrical – RF/Microwave**

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
RF Power - Measure (Relative)	(Ref -30 to 11 dBm) (67 to 110) GHz (-40 to -35) dB (-35 to -30) dB (-30 to -3) dB (-3 to 3) dB (3 to 10) dB (10 to 30) dB	0.18 0.063 0.026 0.0061 0.014 0.023	Comparison to power sensors
RF Power – Measure (Relative)	1 MHz to 2 GHz (Ref -10 to -20 dBm) -60 dBm (-60 to 50) dBm (-50 to 40) dBm (-40 to 30) dBm (-30 to 20) dBm (-20 to 10) dBm (-10 to 5) dBm (-5 to 5) dBm 1.195 GHz (Ref -10 to -22 dBm) (-80 to -79) dBm (-79 to -78) dBm (-78 to -77) dBm (-77 to -76) dBm (-76 to -75) dBm (-75 to -74) dBm (-74 to -73) dBm (-73 to -72) dBm (-72 to -70) dBm (-70 to -69) dBm (-69 to -67) dBm (-67 to -65) dBm (-65 to -60) dBm (-60 to -58) dBm (-58 to -54) dBm (-54 to -50) dBm (-50 to -49) dBm (-49 to -45) dBm (-45 to -40) dBm (-40 to -39) dBm	0.004 9 dB 0.001 5 dB 0.000 84 dB 0.000 76 dB 0.000 23 dB 0.000 097 dB 0.000 11 dB 0.000 32 dB 0.041 dB 0.037 dB 0.035 dB 0.032 dB 0.03 dB 0.029 dB 0.028 dB 0.027 dB 0.026 dB 0.022 dB 0.021 dB 0.02 dB 0.019 dB 0.016 dB 0.015 dB 0.014 dB 0.013 dB 0.012 dB 0.011 dB 0.009 7 dB	Comparison to a Keysight network analyzer, power sensor and signal source



ANSI National Accreditation Board

Electrical – RF/Microwave

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
RF Power – Measure (Relative)	1.195 GHz (Ref -10 to -22 dBm)		Comparison to a Keysight network analyzer, power sensor and signal source
	(-39 to -38) dBm	0.009 1 dB	
	(-38 to -37) dBm	0.008 7 dB	
	(-37 to -35) dBm	0.008 2 dB	
	(-35 to -31) dBm	0.007 9 dB	
	(-31 to -30) dBm	0.007 8 dB	
	(-30 to -29) dBm	0.006 6 dB	
	(-29 to -28) dBm	0.005 7 dB	
	(-28 to -27) dBm	0.005 1 dB	
	(-27 to -26) dBm	0.004 6 dB	
	(-26 to -24) dBm	0.004 1 dB	
	(-24 to -21) dBm	0.003 8 dB	
	(-21 to 1) dBm	0.003 7 dB	
	(1 to 10) dBm	0.005 3 dB	
	1.998 77 GHz		
	(Ref -20 dBm)		
	(-60 to -57) dBm	0.007 1 dB	
	(-57 to -52) dBm	0.006 7 dB	
	(-52 to -49) dBm	0.006 3 dB	
	(-49 to -47) dBm	0.006 dB	
	(-47 to -46) dBm	0.005 8 dB	
	(-46 to -44) dBm	0.005 4 dB	
	(-44 to -42) dBm	0.005 dB	
	(-42 to -41) dBm	0.004 8 dB	
	(-41 to -39) dBm	0.004 5 dB	
	(-39 to -37) dBm	0.004 1 dB	
	(-37 to -35) dBm	0.003 8 dB	
	(-35 to -33) dBm	0.003 5 dB	
	(-33 to -31) dBm	0.003 2 dB	
	(-31 to -29) dBm	0.003 dB	
	(-29 to -27) dBm	0.002 7 dB	
	(-27 to -26) dBm	0.002 5 dB	
	(-26 to -25) dBm	0.002 3 dB	
	(-25 to -23) dBm	0.001 9 dB	
(-23 to -22) dBm	0.001 6 dB		
(-22 to -19) dBm	0.001 dB		
(-19 to -14) dBm	0.002 3 dB		
(-14 to -9) dBm	0.003 3 dB		



ANSI National Accreditation Board

Electrical – RF/Microwave

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
RF Power – Measure (Relative)	1.998 77 GHz (Ref -20 dBm) (-9 to -4) dBm (-4 to 1) dBm (1 to 5) dBm	0.003 9 dB 0.004 7 dB 0.005 7 dB	Comparison to a Keysight network analyzer, power sensor and signal source
RF Power Sensor - Linearity	50 MHz - 37 dBm (-36 to -30) dBm (-30 to -22) dBm (-22 to -15) dBm (-15 to -11) dBm (-11 to 0) dBm (0 to 9) dBm (9 to 13) dBm (13 to 18) dBm (18 to 21) dBm (21 to 26) dBm (26 to 30) dBm	0.39 % of reading 0.24 % of reading 0.2 % of reading 0.16 % of reading 0.12 % of reading 0.1 % of reading 0.061 % of reading 0.1 % of reading 0.11 % of reading 0.12 % of reading 0.33 % of reading 0.34 % of reading	Comparison to a Keysight network analyzer
Dynamic Range	(47 to 220 GHz) (80 to 130) dB	2.7 dB	Comparison to a Keysight network analyzer, millimeter wave test set
Amplitude Flatness - Measure	0.1 V to 8 V 10 kHz to 10 MHz (10 to 50) MHz 50 MHz (50 to 80) MHz 0.1 V to 5.5 V (80 to 300) MHz (0.3 to 1.1) GHz 0.01 V to 0.1 V (50 to 80) MHz (80 to 300) MHz (0.3 to 1.1) GHz	0.025 dB 0.028 dB 0.018 dB 0.023 dB 0.023 dB 0.033 dB 0.027 dB 0.032 dB 0.034 dB	Comparison to a power sensor AC measurement standard and a Keysight 3458A multimeter
Amplitude Modulation Distortion - Measure	500 kHz to 50 GHz (0.01 to 0.1) % Distortion (0.1 to 0.3) % Distortion (0.3 to 15) % Distortion	0.52% of reading + 0.001 1 % Distortion 1% of reading + 0.000 63 % Distortion 1.2 % distortion	Comparison to a Keysight signal analyzer

**Electrical – RF/Microwave**

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Frequency Modulation – Measure	2 MHz to 3.6 GHz (0.2 to 100) (100 to 2 000)	0.35 % of reading + 0.2 %M 0.8 %M	Comparison to a Keysight signal analyzer
	(3.6 to 8.4) GHz (0.2 to 100) (100 to 2 000)	0.7 % of reading + 0.2 %M 2 %M	
	(8.4 to 17.1) GHz (0.2 to 100) (100 to 2 000)	0.7 % of reading + 0.3 %M 2.5 %M	
	(17.1 to 34.5) GHz (0.2 to 100) (100 to 2 000)	0.8 % of reading + 0.3 %M 3 %M	
	(34.5 to 50) GHz (0.2 to 100) (100 to 2 000)	1.4 % of reading + 0.5 %M 4 %M	
Frequency Modulation Distortion - Measure	500 kHz to 50 GHz (0.01 to 15) % Distortion	2.3 % Distortion	Comparison to a Keysight signal analyzer
Phase Modulation Distortion - Measure	500 kHz to 50 GHz (0.01 to 15) % Distortion	2.3 % Distortion	Comparison to a Keysight signal analyzer
Phase Modulation – Measure	(0.2 to 1) rad		Comparison to a Keysight signal analyzer
	100 kHz to 3.6 GHz (3.6 to 17.1) GHz	0.1% of reading + 0.001 rad 0.1% of reading + 0.002 rad	
	(17.1 to 34.5) GHz (34.5 to 50) GHz	0.1% of reading + 0.002 5 rad 0.1% of reading + 0.004 9 rad	
	(1 to 10) rad		
	100 kHz to 3.6 GHz (3.6 to 17.1) GHz (17.1 to 34.5) GHz (34.5 to 50) GHz	0.008 1 % of reading + 0.002 rad 0.015 % of reading + 0.003 rad 0.02 % of reading + 0.003 5 rad 0.058 % of reading + 0.005 8 rad	
Phase Modulation Frequency Response - Measure	80 Hz to 100 kHz Deviation 4 rad	0.057 dB	Comparison to a Keysight signal analyzer and a Keysight 3458A multimeter
	100 Hz to 100 kHz Deviation 1 rad	0.14 dB	



ANSI National Accreditation Board

Electrical – RF/Microwave

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Digital Modulation – Measure GSM EDGE	(0.46 to 2.7) GHz EDGE: residual EVM (0 to 1.5) % GSM: residual phase (0 to 1)° GSM: peak phase (0 to 3)°	0.015 %EVM  0.01°  0.12°	Comparison to a Keysight signal analyzer
Digital Modulation – Measure CDMA2000 IS95 1xEV-DO	Residual EVM (0 to 2) % EVM (0.8 to 2.1) GHz	0.023 % EVM	Comparison to a Keysight signal analyzer
Digital Modulation – Measure W-CDMA	Residual EVM (0 to 2) % EVM (0.8 to 2.2) GHz	0.025 % EVM	Comparison to a Keysight signal analyzer
Digital Modulation – Measure BPSK	Residual EVM (0 to 2.5) % EVM ≤ 3 GHz (3 to 32) GHz (32 to 44) GHz	0.02 % EVM 0.055 % EVM 0.07 % EVM	Comparison to a Keysight signal analyzer
Digital Modulation – Measure QPSK	Residual EVM (0 to 2.5) % EVM ≤ 3 GHz (3 to 6) GHz (6 to 32) GHz (32 to 44) GHz	0.02 % EVM 0.026 % EVM 0.05 % EVM 0.065 % EVM	Comparison to a Keysight signal analyzer
Digital Modulation – Measure $\pi/4$ DQPSK	Residual EVM (0 to 2.5) % EVM ≤ 1 GHz (1 to 2) GHz (2 to 3) GHz (3 to 4) GHz (4 to 6) GHz	0.025 % EVM 0.046 % EVM 0.059 % EVM 0.11 % EVM 0.059 % EVM	Comparison to a Keysight signal analyzer
Digital Modulation – Measure 16, 64 and 256 QAM	Residual EVM (0 to 2.5) % EVM ≤ 3 GHz (3 to 6) GHz (6 to 32) GHz (32 to 44) GHz	0.015 % EVM 0.017 % EVM 0.03 % EVM 0.045 % EVM	Comparison to a Keysight signal analyzer

**Electrical – RF/Microwave**

El Segundo, CA

<b>Parameter/Equipment</b>	<b>Range</b>	<b>Expanded Uncertainty of Measurement (+/-)</b>	<b>Reference Standard, Method, and/or Equipment</b>
Digital Modulation – Measure 2FSK (including DECT)	Shift Error or Deviation (0 to 4) % EVM ≤ 3 GHz (3 to 6) GHz (0 to 10) kHz DECT - kHz	0.049 % 0.048 %  0.12 % of deviation	Comparison to a Keysight signal analyzer
Digital Modulation – Measure NADC	Residual EVM (0 to 2) % EVM (350 to 950) MHz	0.042 % EVM	Comparison to a Keysight signal analyzer
Digital Modulation – Measure PDC	Residual EVM (0 to 2) % EVM (350 to 1501) MHz	0.055 % EVM	Comparison to a Keysight signal analyzer
Digital Modulation – Measure PHS	Residual EVM (0 to 2) % EVM (0.35 to 2) GHz	0.035 % EVM	Comparison to a Keysight signal analyzer
Digital Modulation – Measure TETRA	Residual EVM (0 to 2) % EVM 350 MHz to 1 GHz	0.044 % EVM	Comparison to a Keysight signal analyzer
CISPR Quasi-Peak Absolute Amplitude	Band A, B, C	0.28 dB	Comparison to pulse generator
CISPR Quasi-Peak Detector Variation	Band A, B, C, D	0.12 dB	Comparison to pulse generator
CISPR Response to Pulses Peak Detector	Band A, B Band C, D	0.33 dB 0.3 dB	Comparison to pulse generator
CISPR Response to Pulses Average Detector	Band A Band B Band C, D	0.33 dB 0.35 dB 0.32 dB	Comparison to pulse generator
Distortion Measure	20 Hz to 20 kHz (20 to 100) kHz	1.2 dB 2.4 dB	Comparison to an audio analyzer
Excess Noise Ratio - Measure	(5 to 22) dB (0.01 to 8) GHz (8 to 18) GHz (18 to 28) GHz (28 to 40) GHz (40 to 50) GHz	0.055 dB 0.035 dB 0.059 dB 0.078 dB 0.089 dB	Comparison to a noise source

**Electrical – RF/Microwave**

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Excess Noise Ratio - Measure Cold Source Method	(5 to 22) dB		Comparison to a Keysight network analyzer, and a power Sensor
	(0.5 to 6) GHz	0.1 dB	
	(6 to 18) GHz	0.11 dB	
	(18 to 26.5) GHz	0.13 dB	
	(26.5 to 33) GHz	0.14 dB	
	(33 to 36) GHz	0.15 dB	
	(36 to 39) GHz	0.16 dB	
	(39 to 40) GHz	0.17 dB	
	(40 to 48) GHz	0.2 dB	
	(48 to 50) GHz	0.21 dB	
	(50 to 60) GHz	0.27 dB	
	(60 to 64) GHz	0.29 dB	
(64 to 65) GHz	0.31 dB		
(65 to 67) GHz	0.29 dB		
Phase Noise – Measure	50 kHz to 54 GHz ≥ -187 dBc/Hz		Comparison to a phase noise measurement system
	≤ 10 Hz	2 dB	
	≤ 1 MHz	1.8 dB	
	≤ 100 MHz	3.6 dB	
Phase Noise – Source	1 GHz ≥ -167 dBc/Hz		Comparison to an ultra-low noise reference source
	(10 to 100) Hz	0.5 dB	
	(0.1 to 100) kHz	0.36 dB	
	(0.1 to 1) MHz	0.48 dB	
	(1 to 10) MHz	0.53 dB	
Phase Noise – Source	70 MHz to 1 GHz		Comparison to a low noise signal generator
	>-105 dBc/Hz	0.37 dB	
	>-120 dBc/Hz	0.37 dB	
	>-130 dBc/Hz	0.37 dB	
	>-130 dBc/Hz	0.4 dB	
	> -145 dBc/Hz	0.40 dB	
Noise Voltage - Measure	20 MHz or 1 GHz peak to peak		Comparison to a differential amplifier and a voltmeter
	(>0 to 2) mV	0.07 mV	
	2 mV to 2 V	1.9 % of reading	
	20 MHz rms		
	(>0 to 0.5) mV	21 % of reading	
	(0.5 to 1) mV	6.6 % of reading	
1 mV to 1 V	1.9 % of reading		



ANSI National Accreditation Board

Electrical – RF/Microwave

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Noise Current - Measure	20 MHz rms Up to 10 $\mu$ A (10 to 100) $\mu$ A (0.1 to 250) mA	33 mA/A + 5.7 $\mu$ A 0.11 A/A + 4.2 $\mu$ A 0.15 A/A	Comparison to an oscilloscope and a current probe
Antenna Gain			Comparison to Keysight network analyzer, 8530A Receiver, 8517B S-Parameter Test Set, V85104A, W85104A Modules, Scientific Atlanta 12-2.9, 12-5.8, 12-8.2, 12-12, 12-18, 12-26, 12-33
On Axis Gain, Antenna factor	(5 to 25) dB (0.2 to 26.5) GHz (26.5 to 40) GHz (33 to 50) GHz (50 to 75) GHz (75 to 110) GHz (140 to 220) GHz	0.15 dB 0.2 dB 0.2 dB 0.25 dB 0.3 dB 0.5 dB	Narda 642, 643, 645 TRG 861B/383, Ab90 FXR M638A
Dish Antenna	(5 to 45) dB (12.4 to 110) GHz	0.31 dB	Hughes 45826H-1020 TRG/Custom Microwave Wr-5 Gain Horns, X, Ku, K, Ka, Q, V, W Probes Leica LT300 Laser Tracker
Directional/ SWR Bridge Reflections/ Directivity	(0 to 60) dB 5 Hz to 110 GHz	0.03 $\Gamma$ 1 dB	Comparison to Agilent/HP 8757D Network Analyzer, 355C/D Step Attenuators, 85054B Calibration Kit, 8481D opt H70, 8487A, VA8486A, W8486
Insertion Loss/Linearity	(0 to 60) dB 5 Hz to 67 GHz (67 to 110) GHz	0.1 dB 0.1 dB	Power Sensors, E8361C Network Analyzer, V85104A, W85104A Modules



ANSI National Accreditation Board

Electrical – RF/Microwave

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Directional Coupler Main Line Loss	5 Hz to 67 GHz	0.1 dB	Comparison to Agilent/HP E8361A Network Analyzer, 8510C Network Analyzer, 8517B S-Parameter Test Set V85104A, W85104A Modules, E8361C Network Analyzer, 85054B Calibration Kit, TRL Calibration Kit
Coupling Loss	(67 to 110) GHz	0.2 dB	
Reflection	5 Hz to 67 GHz	0.1 dB	
Directivity	(67 to 110) GHz	0.2 dB	
Gaussian Noise	(-100 to +20) dBm	0.05 dB	Comparison to Agilent/HP 8482A/D, 8481A/D, 8485A/D, 8487 A/D Power Sensors, Agilent/HP 8565E Spectrum Analyzer
Noise Output Power	100 kHz to 18 GHz	0.11 dB	
Signal Path Response	(-60 to +20) dB	1 dB	Comparison to Agilent E4448A Spectrum Analyzer
	9 kHz to 3 GHz	2.6 dB	
	(3 to 22) GHz	3.5 dB	
Gaussian Noise Attenuation	(0 to 10) dB	0.1 dB	Comparison to Agilent E4448A Spectrum Analyzer
	(10 to 30) dB	0.2 dB	
	(40 to 50) dB	0.3 dB	
Harmonic Mixer Conversion Loss	(0 to 50) dB	1.8 dB	Comparison to Agilent/HP 8563E Spectrum Analyzer, 8485A, 8487A, V8486A, W8486A Power Sensors Hughes/HP/Millitech Thermistor mounts
	(18 to 26.5) GHz	1.8 dB	
	(26.5 to 40) GHz	1.8 dB	
	(33 to 50) GHz	1.8 dB	
	(50 to 75) GHz	1.8 dB	
RF Power – Absolute	(-30 to +20) dBm	1.1 % of reading	Comparison to Hughes/Millitech/Agilent/HP Thermistor Mounts, V8486A, W8486A, E4419B
WR-42	(18 to 26.5) GHz	1.1 % of reading	
WR-28	(26.5 to 40) GHz	1.5 % of reading	
WR-22	(33 to 50) GHz	2 % of reading	
WR-15	(50 to 75) GHz	2.5 % of reading	
WR-10	(75 to 110) GHz		



ANSI National Accreditation Board

Electrical – RF/Microwave

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Power Sensor Characterization Waveguide			
S Band	(2.6 to 3.95) GHz	0.9 dB	Comparison to Waveguide Thermistor/ Thermocouple or Diode Power Sensors
G Band	(3.95 to 5.85) GHz	0.9 dB	
H Band	(7.05 to 10) GHz	0.9 dB	
X Band	(8.2 to 12.4) GHz	1.1 dB	
Ku band	(12.4 to 18) GHz	1.1 dB	
K Band	(18 to 26.5) GHz	1.2 dB	
Ka Band	(26.5 to 40) GHz	1.1 % of reading	
Q Band	(33 to 50) GHz	1.8 % of reading	
Power Sensor Characterization V Band	(50 to 52) GHz (52 to 56) GHz (56 to 64) GHz (65 to 75) GHz	2.5 % of reading 2.4 % of reading 2.7 % of reading 2.4 % of reading	Comparison to Waveguide Thermistor/ Thermocouple or Diode Power Sensors
Power Sensor Characterization W Band	(75 to 76) GHz (76 to 77) GHz (77 to 80) GHz (80 to 81) GHz (81 to 110) GHz	3.2 % of reading 3 % of reading 2.9 % of reading 4.6 % of reading 3.1 % of reading	Comparison to Waveguide Thermistor/ Thermocouple or Diode Power Sensors
Power Sensor Characterization (75 Ω)	100 kHz to 2 GHz (2 to 4.2) GHz	1.3 % of reading 1.5 % of reading	Comparison to Tegam F1119, Tegam 1804 Power Standards, NIST CN Mount, Agilent 11852B

**Electrical – RF/Microwave**

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Scattering Parameters Waveguide Reflection: S11 and S22 Reflection Coefficient	(2.6 to 12.4) GHz (0 to 1) lin (-180 to 180)°	0.009 0.5°	Comparison to Agilent/HP 8510C Network Analyzer, 8517B S-Parameter Test Set, E8361A Network Analyzer, V85104A, W85104A Modules. PSNA TRL Calibration Kit, Oleson V05 VNA1-T/R WR28 S-Parameter Ref Standards WR22 S-Parameter Ref Standards WR15 S-Parameter Ref Standards WR10 S-Parameter Ref Standards
	(12.4 to 26.5) GHz (0 to 1) lin (-180 to 180)°	0.01 0.5°	
	(26.5 to 50) GHz (0 to 1) lin (-180 to 180)°	0.006 0.3°	
	(50 to 75) GHz (0 to 1) lin (-180 to 180)°	0.018 1.1°	
	(75 to 110) GHz (0 to 1) lin (-180 to 180)°	0.024 1.4°	
	(140 to 220) GHz (0 to 1) lin (-180 to 180)°	0.048 10°	

Electrical – RF/Microwave

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Scattering Parameters Waveguide	(2.6 to 12.4) GHz		Comparison to Agilent/HP 8510C Network Analyzer, 8517B S-Parameter Test Set, E8361A Network Analyzer, V85104A, W85104A Modules, PSNA TRL Calibration Kit, Oleson V05 VNA1-T/R WR28 S-Parameter Ref Standards WR22 S-Parameter Ref Standards WR15 S-Parameter Ref Standards WR10 S-Parameter Ref Standards
	(0 to 30) dB	0.02 dB	
	(-180 to 180)°	0.6°	
	(30 to 50) dB	0.08 dB	
	(-180 to 180) °	0.7°	
	(0 to 30) dB	0.02 dB	
	(-180 to 180)°	0.7°	
	(12.4 to 18) GHz		
	(30 to 50) dB	0.09 dB	
	(-180 to 180)°	0.7°	
	(0 to 30) dB	0.05 dB	
	(-180 to 180)°	1.8°	
	(18 to 26.5) GHz		
	(30 to 50) dB	0.08 dB	
	(-180 to 180)°	1.8°	
(0 to 30) dB	0.03 dB		
(-180 to 180)°	1.2°		
(26.5 to 40) GHz			
(30 to 50) dB	0.09 dB		
(-180 to 180)°	1.4°		
(0 to 30) dB	0.03 dB		
(-180 to 180)°	1.8°		
Scattering Parameters Waveguide	(40.0 to 50.0) GHz		Comparison to Agilent/HP 8510C Network Analyzer, 8517B S-Parameter Test Set, E8361A Network Analyzer, V85104A, W85104A Modules, PSNA TRL Calibration Kit, Oleson V05 VNA1-T/R WR28 S-Parameter Ref Standards WR22 S-Parameter Ref Standards WR15 S-Parameter Ref Standards WR10 S-Parameter Ref Standards
	(30 to 50) dB	0.09 dB	
	(-180 to 180)°	2.1°	
	(0 to 30) dB	0.05 dB	
	(-180 to 180)°	3.3°	
	(50 to 75.0) GHz		
	(30 to 50) dB	0.1 dB	
	(-180 to 180)°	3.4°	
	(0 to 30) dB	0.06 dB	
	(-180 to 180)°	4.6°	
	(75 to 110) GHz		
	(30 to 50) dB	0.11 dB	
	(-180 to 180)°	5.4°	
	(0 to 30) dB	0.07 dB	
	(-180 to 180)°	9.3°	
(140 to 220) GHz			
(30 to 40) dB	1 dB		
(-180 to 180)°	14°		



ANSI National Accreditation Board

Electrical – RF/Microwave

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Thermal Noise Waveguide (26.5 to 50) GHz	(5 to 30) dB ENR (26.5 to 27) GHz (27 to 31) GHz (31 to 39) GHz 40 GHz (40 to 50) GHz	0.07 dB 0.06 dB 0.08 dB 0.1 dB 0.13 dB	Comparison to Agilent 8970B, 8971C, N8975A, 346C Noise Source, 8510C Network Analyzer, 8517B S-Parameter Test Set, Clare TN162 (WR-28), TN 172 (WR-22), TN164 (WR-15), TN165 (WR-10) Noise Sources
Thermal Noise Waveguide (50 to 75) GHz	(5 to 30) dB ENR (50 to 54) GHz 55 GHz (55 to 63) GHz (63 to 65) GHz 66 GHz 67 GHz 68 GHz 69 GHz 70 GHz 71 GHz 72 GHz 73 GHz 74 GHz 75 GHz	0.15 dB 0.14 dB 0.16 dB 0.19 dB 0.21 dB 0.23 dB 0.25 dB 0.26 dB 0.28 dB 0.31 dB 0.33 dB 0.34 dB 0.34 dB 0.36 dB	Comparison to Agilent 8970B, 8971C, N8975A, 346C Noise Sources, 8510C Network Analyzer, 8517B S-Parameter Test Set, Clare TN162 (WR-28), TN 172 (WR-22), TN164 (WR-15), TN165 (WR-10) Noise Sources
Thermal Noise Waveguide (75 to 110) GHz	(3 to 30) dB ENR (75 to 77) GHz (77 to 80) GHz (80 to 89) GHz (89 to 94) GHz (94 to 100) GHz 101 GHz 102 GHz 103 GHz 104 GHz 105 GHz 106 GHz 107 GHz 108 GHz 109 GHz 110 GHz	0.3 dB 0.31 dB 0.44 dB 0.31 dB 0.43 dB 0.78 dB 0.77 dB 0.77 dB 0.76 dB 0.75 dB 0.94 dB 1.1 dB 1.3 dB 1.5 dB 1.7 dB	Comparison to Agilent 8970B, N8975A, Clare TN164 (WR-15), TN 165 (WR-10) Noise Sources

**Electrical – RF/Microwave**

El Segundo, CA

Parameter/Equipment		Attenuation – Source									
Reference Standard, Method, and/or Equipment		Comparison to an attenuator									
Expanded Uncertainty of Measurement (+/-)											
Range	1 dB	2 dB	3 dB	4 dB	5 dB	6 dB	7 dB	8 dB	9 dB	10 dB	11 dB
20 Hz to 50 MHz	0.0028 dB	0.0028 dB	0.0028 dB	0.0029 dB	0.0029 dB	0.0029 dB	0.0029 dB	0.0029 dB	0.0029 dB	0.0029 dB	0.0029 dB
50 MHz to 1 GHz	0.0053 dB	0.0053 dB	0.0053 dB	0.0053 dB	0.0053 dB	0.0053 dB	0.0053 dB	0.0053 dB	0.0053 dB	0.0054 dB	0.0054 dB
(1 to 2) GHz	0.0063 dB	0.0063 dB	0.0063 dB	0.0063 dB	0.0063 dB	0.0063 dB	0.0063 dB	0.0063 dB	0.0063 dB	0.0063 dB	0.0063 dB
(2 to 4) GHz	0.008 dB	0.008 dB	0.0081 dB	0.0081 dB	0.0081 dB	0.0081 dB	0.0081 dB	0.0081 dB	0.0081 dB	0.0081 dB	0.0081 dB
(4 to 10) GHz	0.013 dB	0.012 dB	0.015 dB	0.014 dB	0.017 dB	0.016 dB	0.015 dB	0.015 dB	0.021 dB	0.013 dB	0.015 dB
(10 to 12.4) GHz	0.021 dB	0.027 dB	0.032 dB	0.027 dB	0.022 dB	0.022 dB	0.019 dB	0.024 dB	0.025 dB	0.036 dB	0.036 dB
(12.4 to 18) GHz	0.034 dB	0.037 dB	0.035 dB	0.033 dB	0.040 dB	0.038 dB	0.035 dB	0.038 dB	0.045 dB	0.042 dB	0.036 dB

**Electrical – RF/Microwave**

El Segundo, CA

Parameter/Equipment		Attenuation – Source									
Reference Standard, Method, and/or Equipment		Comparison to an attenuator									
Expanded Uncertainty of Measurement (+/-)											
Range	10 dB	20 dB	30 dB	40 dB	50 dB	60 dB	70 dB	80 dB	90 dB	100 dB	110 dB
20 Hz to 50 MHz	0.0039 dB	0.0043 dB	0.0075 dB	0.0075 dB	0.0096 dB	0.011 dB	0.016 dB	0.019 dB	0.022 dB	0.032 dB	0.039 dB
50 MHz to 1 GHz	0.0051 dB	0.0048 dB	0.0057 dB	0.0065 dB	0.019 dB	0.022 dB	0.032 dB	0.039 dB	0.045 dB	0.057 dB	0.074 dB
(1 to 2) GHz	0.006 dB	0.0059 dB	0.006 dB	0.0083 dB	0.025 dB	0.029 dB	0.042 dB	0.033 dB	0.058 dB	0.058 dB	0.082 dB
(2 to 4) GHz	0.0075 dB	0.0073 dB	0.0082 dB	0.012 dB	0.034 dB	0.035 dB	0.057 dB	0.035 dB	0.06 dB	0.062 dB	0.086 dB
(4 to 10) GHz	0.01 dB	0.0098 dB	0.01 dB	0.012 dB	0.038 dB	0.038 dB	0.065 dB	0.038 dB	0.065 dB	0.068 dB	0.093 dB
(10 to 12.4) GHz	0.01 dB	0.0099 dB	0.01 dB	0.012 dB	0.038 dB	0.038 dB	0.065 dB	0.038 dB	0.065 dB	0.086 dB	0.12 dB
(12.4 to 18) GHz	0.01 dB	0.0099 dB	0.01 dB	0.012 dB	0.038 dB	0.038 dB	0.065 dB	0.038 dB	0.065 dB	0.17 dB	0.18 dB

**Electrical – RF/Microwave**

El Segundo, CA

Parameter/ Equipment		RF Power - Measure										
Reference Standard, Method, and/or Equipment		Comparison to a power sensor and a Keysight signal analyzer										
Expanded Uncertainty of Measurement (+/-)												
Range	(-140 to -130) dBm	(-130 to -110) dBm	(-110 to -90) dBm	(-90 to -30) dBm	(-30 to -10) dBm	(-10 to -3) dBm	(-3 to +3) dBm	(3 to 14) dBm	(14 to 20) dBm	(20 to 25) dBm	(25 to 35) dBm	(35 to 44) dBm
(0.9 to 9) kHz	-	-	-	-	0.044 dB	0.044 dB	0.027 dB	0.032 dB	0.043 dB	-	-	-
(9 to 100) kHz	0.17 dB	0.17 dB	0.16 dB	0.16 dB	0.044 dB	0.044 dB	0.027 dB	0.032 dB	0.032 dB	0.034 dB	0.036 dB	-
(0.1 to 10) MHz	0.085 dB	0.071 dB	0.054 dB	0.045 dB	0.043 dB	0.042 dB	0.027 dB	0.032 dB	0.032 dB	0.034 dB	0.037 dB	-
50 MHz	0.079 dB	0.066 dB	0.048 dB	0.037 dB	0.034 dB	0.032 dB	0.02 dB	0.027 dB	0.023 dB	0.024 dB	0.029 dB	-
(10 to 100) MHz	0.081 dB	0.068 dB	0.05 dB	0.04 dB	0.038 dB	0.037 dB	0.027 dB	0.029 dB	0.032 dB	0.034 dB	0.036 dB	0.06 dB
(0.1 to 4) GHz	0.080 dB	0.067 dB	0.049 dB	0.039 dB	0.036 dB	0.035 dB	0.024 dB	0.027 dB	0.037 dB	0.038 dB	0.041 dB	0.057 dB
(4 to 8) GHz	0.081 dB	0.068 dB	0.05 dB	0.04 dB	0.038 dB	0.037 dB	0.027 dB	0.032 dB	0.039 dB	0.041 dB	0.043 dB	0.058 dB
(8 to 18) GHz	0.084 dB	0.071 dB	0.053 dB	0.043 dB	0.040 dB	0.039 dB	0.029 dB	0.035 dB	0.038 dB	0.040 dB	0.042 dB	0.06 dB
(18 to 24) GHz	0.091 dB	0.076 dB	0.069 dB	0.050 dB	0.048 dB	0.047 dB	0.031 dB	0.044 dB	0.053 dB	0.061 dB	0.063 dB	-
(24 to 40) GHz	0.12 dB	0.11 dB	0.1 dB	0.091 dB	0.069 dB	0.069 dB	0.059 dB	0.061 dB	0.068 dB	0.069 dB	0.076 dB	-
(40 to 50) GHz	0.13 dB	0.10 dB	0.098 dB	0.085 dB	0.083 dB	0.083 dB	0.079 dB	0.081 dB	0.086 dB	0.11 dB	0.11 dB	-
(50 to 60) GHz	0.17 dB	0.13 dB	0.12 dB	0.10 dB	0.099 dB	0.099 dB	0.093 dB	0.094 dB	0.099 dB	-	-	-
(60 to 67) GHz	0.52 dB	0.22 dB	0.22 dB	0.21 dB	0.099 dB	0.099 dB	0.093 dB	0.094 dB	0.099 dB	-	-	-
(67 to 80) GHz	-	-	-	-	0.26 dB	0.26 dB	0.26 dB	0.26 dB	0.26 dB	-	-	-
(80 to 90) GHz	-	-	-	-	0.32 dB	0.32 dB	0.32 dB	0.32 dB	0.32 dB	-	-	-
(90 to 100) GHz	-	-	-	-	0.3 dB	0.3 dB	0.3 dB	0.3 dB	0.3 dB	-	-	-
(100 to 110) GHz	-	-	-	-	0.29 dB	0.29 dB	0.29 dB	0.29 dB	0.29 dB	-	-	-



ANSI National Accreditation Board

Electrical – RF/Microwave

El Segundo, CA

Parameter/Equipment	Amplitude Modulation Depth - Measure		
Reference Standard, Method, and/or Equipment	Comparison to a Keysight signal analyzer (% indicates % Depth where not specified)		
Frequency Range	AM Depth	Modulation Rate	Expanded Uncertainty of Measurement (+/-)
2 Hz to 50 GHz	(5 to 20) %	10 Hz to 100 kHz	0.11% of reading + 0.0083 %
	(20 to 40) %		0.022% of reading + 0.026 %
	(40 to 50) %		0.0027% of reading + 0.034 %
	(50 to 60) %		-0.013% of reading + 0.043 %
	(60 to 75) %		-0.041% of reading + 0.06 %
	(75 to 90) %		-0.091% of reading + 0.099 %
	(90 to 95) %		0.01 %
	(95 to 98) %		0.0051 %
100 kHz to 13.6 GHz	(5 to 50) %	10 Hz to 25 kHz	0.1% of reading
	(5 to 30) %	(25 to 50) kHz	0.16% of reading
	(5 to 20) %	(50 to 100) kHz	0.22% of reading
	(5 to 95) %	(100 to 250) kHz	0.32% of reading
		(250 to 500) kHz	0.5% of reading
		(0.5 to 1) MHz	0.71% of reading
		1 MHz	1% of reading
(13.5 to 17.1) GHz	(5 to 50) %	10 Hz to 10 kHz	0.1% of reading
	(5 to 35) %	(10 to 25) kHz	0.14% of reading
	(5 to 20) %	(25 to 50) kHz	0.22% of reading
	(5 to 15) %	(50 to 100) kHz	0.32% of reading
	(5 to 95) %	(100 to 250) kHz	0.45% of reading
		(250 to 500) kHz	0.71% of reading
		(0.5 to 1) MHz	1% of reading
		1 MHz	1.4% of reading
(17 to 34.5) GHz	(5 to 50) %	10 Hz to 5 kHz	0.1% of reading
	(5 to 55) %	(5 to 10) kHz	0.095% of reading
	(5 to 30) %	(10 to 25) kHz	0.15% of reading
	(5 to 20) %	(25 to 50) kHz	0.25% of reading
	(5 to 10) %	(50 to 100) kHz	0.36% of reading
	(5 to 95) %	(100 to 250) kHz	0.52% of reading
		(250 to 500) kHz	0.84% of reading
		(0.5 to 1) MHz	1.2% of reading
		1 MHz	1.7% of reading
(34.4 to 50) GHz	(5 to 15) %	10 Hz to 5 kHz	0.25% of reading
	(5 to 15) %	(5 to 10) kHz	0.31% of reading
	(5 to 10) %	(10 to 25) kHz	0.37% of reading
	(5 to 95) %	(100 to 250) kHz	1.5% of reading
		(250 to 500) kHz	3.3% of reading
		(0.5 to 1) MHz	6.3% of reading
		1 MHz	12% of reading

**Electrical – RF/Microwave**

El Segundo, CA

Parameter/Equipment		Frequency Modulation Deviation - Measure		
Reference Standard, Method, and/or Equipment		Comparison to a Keysight signal analyzer		
Frequencies	Deviation Range	Modulation Rate	Modulation index	Expanded Uncertainty of Measurement (+/-)
100 kHz to 3.6 GHz	20 Hz to 2 MHz	10 Hz to 500 kHz	$\beta \geq 0.5$	0.2 % of reading
100 kHz to 3.6 GHz	10 Hz to 10 MHz	20 Hz to 1 MHz	$\beta \geq 0.2$	0.7 % of reading
100 kHz to 3.6 GHz	10 Hz to 16 MHz	50 Hz to 1 MHz	$\beta \geq 0.05$	2 % of reading
100 kHz to 3.6 GHz	10 Hz to 50 kHz	100 Hz to 1 MHz	$\beta \geq 0.025$	5.2 % of reading
100 kHz to 3.6 GHz	10 Hz to 40 kHz	100 Hz to 1 MHz	$\beta \geq 0.02$	10 % of reading
100 kHz to 3.6 GHz	10 Hz to 20 kHz	500 Hz to 1 MHz	$\beta \geq 0.01$	20 % of reading
(3.5 to 8.4) GHz	20 Hz to 1 MHz	10 Hz to 500 kHz	$\beta \geq 0.5$	0.21 % of reading
(3.5 to 8.4) GHz	10 Hz to 5 MHz	20 Hz to 1 MHz	$\beta \geq 0.2$	0.7 % of reading
(3.5 to 8.4) GHz	10 Hz to 16 MHz	50 Hz to 1 MHz	$\beta \geq 0.05$	2.2 % of reading
(3.5 to 8.4) GHz	10 Hz to 16 MHz	100 Hz to 1 MHz	$\beta \geq 0.025$	5.2 % of reading
(3.5 to 8.4) GHz	10 Hz to 40 kHz	100 Hz to 1 MHz	$\beta \geq 0.02$	10 % of reading
(3.5 to 8.4) GHz	10 Hz to 20 kHz	500 Hz to 1 MHz	$\beta \geq 0.01$	20 % of reading
(8.3 to 13.6) GHz	20 Hz to 2 MHz	10 Hz to 500 kHz	$\beta \geq 0.5$	0.21 % of reading
(8.3 to 13.6) GHz	10 Hz to 10 MHz	50 Hz to 1 MHz	$\beta \geq 0.2$	0.7 % of reading
(8.3 to 13.6) GHz	10 Hz to 16 MHz	50 Hz to 1 MHz	$\beta \geq 0.05$	2.2 % of reading
(8.3 to 13.6) GHz	10 Hz to 500 kHz	100 Hz to 1 MHz	$\beta \geq 0.025$	5.2 % of reading
(8.3 to 13.6) GHz	10 Hz to 40 kHz	100 Hz to 1 MHz	$\beta \geq 0.02$	10 % of reading
(8.3 to 13.6) GHz	10 Hz to 20 kHz	500 Hz to 1 MHz	$\beta \geq 0.01$	20 % of reading
(13.5 to 17.1) GHz	20 Hz to 1 MHz	10 Hz to 200 kHz	$\beta \geq 0.5$	0.21 % of reading
(13.5 to 17.1) GHz	10 Hz to 5 MHz	20 Hz to 1 MHz	$\beta \geq 0.2$	0.7 % of reading
(13.5 to 17.1) GHz	10 Hz to 16 MHz	50 Hz to 1 MHz	$\beta \geq 0.05$	2.2 % of reading
(13.5 to 17.1) GHz	10 Hz to 16 MHz	100 Hz to 1 MHz	$\beta \geq 0.025$	5.2 % of reading
(13.5 to 17.1) GHz	10 Hz to 40 kHz	100 Hz to 1 MHz	$\beta \geq 0.02$	10 % of reading
(13.5 to 17.1) GHz	10 Hz to 20 kHz	500 Hz to 1 MHz	$\beta \geq 0.01$	20 % of reading
(17 to 26.5) GHz	50 Hz to 400 kHz	10 Hz to 50 kHz	$\beta \geq 0.8$	0.31 % of reading
(17 to 26.5) GHz	20 Hz to 5 MHz	10 Hz to 1 MHz	$\beta \geq 0.2$	0.9 % of reading
(17 to 26.5) GHz	20 Hz to 10 MHz	100 Hz to 1 MHz	$\beta \geq 0.08$	3.3 % of reading
(17 to 26.5) GHz	10 Hz to 16 MHz	100 Hz to 1 MHz	$\beta \geq 0.04$	6.3 % of reading
(17 to 26.5) GHz	10 Hz to 40 kHz	100 Hz to 1 MHz	$\beta \geq 0.02$	12 % of reading
(17 to 26.5) GHz	10 Hz to 1 kHz	500 Hz to 100 kHz	$\beta \geq 0.01$	30 % of reading
(26.4 to 34.5) GHz	50 Hz to 400 kHz	10 Hz to 50 kHz	$\beta \geq 0.8$	0.31 % of reading

**Electrical – RF/Microwave**

El Segundo, CA

Parameter/Equipment		Frequency Modulation Deviation - Measure		
Reference Standard, Method, and/or Equipment		Comparison to a Keysight signal analyzer		
Frequencies	Deviation Range	Modulation Rate	Modulation index	Expanded Uncertainty of Measurement (+/-)
(26.4 to 34.5) GHz	20 Hz to 5 MHz	10 Hz to MHz	$\beta \geq 0.2$	0.9 % of reading
(26.4 to 34.5) GHz	20 Hz to 10 MHz	100 Hz to 1 MHz	$\beta \geq 0.08$	3.3 % of reading
(26.4 to 34.5) GHz	10 Hz to 16 MHz	100 Hz to 1 MHz	$\beta \geq 0.04$	6.3 % of reading
(26.4 to 34.5) GHz	10 Hz to 16 MHz	100 Hz to 1 MHz	$\beta \geq 0.02$	12 % of reading
(26.4 to 34.5) GHz	10 Hz to 1 kHz	500 Hz to 100 kHz	$\beta \geq 0.01$	30 % of reading
(34.4 to 50) GHz	50 Hz to 100 kHz	10 Hz to 20 kHz	$\beta \geq 0.8$	0.32 % of reading
(34.4 to 50) GHz	20 Hz to 500 kHz	10 Hz to 200 kHz	$\beta \geq 0.2$	0.9 % of reading
(34.4 to 50) GHz	20 Hz to 2 MHz	20 Hz to 1 MHz	$\beta \geq 0.08$	3.3 % of reading
(34.4 to 50) GHz	10 Hz to 5 MHz	50 Hz to 1 MHz	$\beta \geq 0.04$	6.4 % of reading
(34.4 to 50) GHz	10 Hz to 16 MHz	100 Hz to 1 MHz	$\beta \geq 0.02$	12 % of reading
(34.4 to 50) GHz	10 Hz to 16 MHz	500 Hz to 200 kHz	$\beta \geq 0.01$	30 % of reading

**Electrical - RF Microwave**

El Segundo, CA

Parameter/Equipment		Voltage Reflection Coefficient S11/S22 - Magnitude <sup>3</sup>								
Reference Standard, Method, and/or Equipment		Comparison to a Keysight network analyzer								
Expanded Uncertainty of Measurement (+/-)										
Range	0 to 0.1	0.1 to 0.2	0.2 to 0.3	0.3 to 0.4	0.4 to 0.5	0.5 to 0.6	0.6 to 0.7	0.7 to 0.8	0.8 to 0.9	0.9 to 1.0
DC to 10 MHz	0.000 17	0.000 23	0.000 3	0.000 37	0.000 41	0.000 45	0.000 48	0.000 51	0.000 53	0.000 22
10 MHz to 2 GHz	0.000 18	0.000 23	0.000 31	0.000 38	0.000 43	0.000 47	0.000 5	0.000 52	0.000 53	0.000 22
(2 to 8) GHz	0.000 56	0.000 61	0.000 71	0.000 76	0.000 75	0.000 72	0.000 66	0.000 59	0.000 55	0.000 23
(8.0 to 20) GHz	0.000 56	0.000 61	0.000 7	0.000 8	0.000 9	0.001	0.000 97	0.000 94	0.000 94	0.000 89
(20 to 26.5) GHz	0.000 89	0.000 96	0.001 1	0.001 2	0.001 4	0.001 6	0.001 5	0.001 4	0.001 4	0.001 4
(26.5 to 33) GHz	0.000 89	0.000 98	0.001 2	0.001 4	0.001 7	0.001 8	0.001 6	0.001 5	0.001 4	0.001 4
(33 to 40) GHz	0.000 9	0.000 99	0.001 2	0.001 5	0.001 7	0.002	0.001 8	0.001 6	0.001 5	0.001 5
(40 to 45) GHz	0.001 4	0.001 5	0.001 7	0.001 9	0.002 1	0.002 4	0.002 3	0.002 1	0.002 1	0.002 1
(45 to 50) GHz	0.001 4	0.001 5	0.001 7	0.001 8	0.002	0.002 2	0.002 4	0.002 3	0.002 1	0.002 1
(50 to 60) GHz	0.002 5	0.002 6	0.002 8	0.003 1	0.003 4	0.003 7	0.004	0.004 3	0.004 7	0.005 3
(60 to 67) GHz	0.002 5	0.002 7	0.002 9	0.003 2	0.003 7	0.004 2	0.004 7	0.005 1	0.005 7	0.006 4
(67 to 75) GHz	0.005 4	0.005 9	0.006 1	0.006 3	0.006 5	0.006 8	0.007 1	0.007 5	0.007 8	0.008 2

**Electrical - RF Microwave**

El Segundo, CA

<b>Parameter/Equipment</b>	Voltage Reflection Coefficient S11/S22 - Magnitude <sup>3</sup>									
<b>Reference Standard, Method, and/or Equipment</b>	Comparison to a Keysight network analyzer									
<b>Expanded Uncertainty of Measurement (+/-)</b>										
(75 to 110) GHz	0.003 5	0.004	0.004 2	0.004 6	0.004 9	0.005 3	0.005 8	0.006 3	0.006 9	0.007 5
(110 to 120) GHz	0.03	0.033	0.036	0.039	0.04	0.047	0.052	0.057	0.063	0.07

**Electrical - RF Microwave**

<b>Parameter/Equipment</b>	Voltage Reflection Coefficient S11/S22 – Phase									
<b>Reference Standard, Method, and/or Equipment</b>	Comparison to a Keysight network analyzer									
<b>Expanded Uncertainty of Measurement (+/-)</b>										
<b>Range</b>	0 to 0.1	0.1 to 0.2	0.2 to 0.3	0.3 to 0.4	0.4 to 0.5	0.5 to 0.6	0.6 to 0.7	0.7 to 0.8	0.8 to 0.9	0.9 to 1.0
DC to 10 MHz	0.13°	0.086°	0.070°	0.059°	0.052°	0.046°	0.041°	0.038°	0.035°	0.013°
10 MHz to 2 GHz	0.13°	0.089°	0.073°	0.062°	0.054°	0.048°	0.043°	0.038°	0.035°	0.013°
(2.0 to 8.0) GHz	0.37°	0.22°	0.16°	0.12°	0.094°	0.076°	0.063°	0.05°	0.042°	0.026°
(8.0 to 20) GHz	0.39°	0.26°	0.21°	0.16°	0.13°	0.11°	0.092°	0.081°	0.071°	0.065°
(20 to 26.5) GHz	0.58°	0.40°	0.36°	0.29°	0.23°	0.2°	0.17°	0.16°	0.15°	0.15°
(26.5 to 33) GHz	0.57°	0.36°	0.31°	0.0°	0.29°	0.23°	0.19°	0.16°	0.14°	0.14°
(33 to 40) GHz	0.58°	0.39°	0.34°	0.32°	0.29°	0.24°	0.19°	0.16°	0.14°	0.13°
(40 to 45) GHz	0.86°	0.50°	0.39°	0.34°	0.32°	0.31°	0.31°	0.27°	0.26°	0.26°
(45 to 50) GHz	0.88°	0.55°	0.46°	0.43°	0.42°	0.36°	0.31°	0.28°	0.26°	0.26°
(50 to 60) GHz	1.5°	0.82°	0.63°	0.55°	0.52°	0.51°	0.52°	0.53°	0.5°	0.47°
(60 to 67) GHz	1.5°	0.84°	0.65°	0.58°	0.55°	0.54°	0.54°	0.53°	0.5°	0.47°
(67 to 75) GHz	3.2°	1.7°	1.2°	0.90°	0.75°	0.65°	0.58°	0.53°	0.5°	0.47°
(75 to 110) GHz	2.1°	1.1°	0.81°	0.65°	0.57°	0.51°	0.48°	0.45°	0.44°	0.43°
(110 to 120) GHz	18°	9.6°	6.9°	5.6°	4.9°	4.5°	4.3°	4.1°	4.0°	4.0°

**Electrical - RF Microwave**

El Segundo, CA

Parameter/Equipment		Transmission S12/S21 – Magnitude							
Reference Standard, Method, and/or Equipment		Comparison to a Keysight network analyzer							
Expanded Uncertainty of Measurement (+/-)									
Range	(0 to 3) dB	(3 to 6) dB	(6 to 10) dB	(10 to 20) dB	(20 to 30) dB	(30 to 40) dB	(40 to 50) dB	(50 to 60) dB	(60 to 70) dB
DC to 10 MHz	0.000 57 dB	0.005 8 dB	0.007 3 dB	0.009 3 dB	0.013 dB	0.017 dB	0.02 dB	0.026 dB	0.044 dB
10 MHz to 2 GHz	0.000 3 dB	0.005 3 dB	0.006 1 dB	0.007 2 dB	0.01 dB	0.014 dB	0.017 dB	0.021 dB	0.028 dB
(2.0 to 8.0) GHz	0.000 3 dB	0.005 3 dB	0.006 1 dB	0.007 2 dB	0.01 dB	0.014 dB	0.017 dB	0.021 dB	0.028 dB
(8.0 to 20) GHz	0.000 3 dB	0.005 3 dB	0.006 1 dB	0.007 2 dB	0.01 dB	0.015 dB	0.018 dB	0.021 dB	0.026 dB
(20 to 26.5) GHz	0.009 3 dB	0.01 dB	0.011 dB	0.012 dB	0.014 dB	0.016 dB	0.019 dB	0.022 dB	0.027 dB
(26.5 to 33) GHz	0.014 3 dB	0.015 dB	0.015 dB	0.016 dB	0.017 dB	0.019 dB	0.022 dB	0.028 dB	0.051 dB
(33 to 40) GHz	0.020 1 dB	0.021 dB	0.021 dB	0.021 dB	0.022 dB	0.026 dB	0.031 dB	0.036 dB	0.056 dB
(40 to 45) GHz	0.022 dB	0.022 dB	0.023 dB	0.023 dB	0.024 dB	0.028 dB	0.037 dB	0.044 dB	0.08 dB
(45 to 50) GHz	0.023 1 dB	0.024 dB	0.024 dB	0.024 dB	0.025 dB	0.029 dB	0.037 dB	0.045 dB	0.08 dB
(50 to 60) GHz	0.027 9 dB	0.028 dB	0.028 dB	0.029 dB	0.03 dB	0.031 dB	0.033 dB	0.042 dB	0.085 dB
(60 to 67) GHz	0.034 dB	0.034 dB	0.034 dB	0.035 dB	0.035 dB	0.037 dB	0.039 dB	0.048 dB	0.096 dB
(67 to 75) GHz	0.043 dB	0.046 dB	0.048 dB	0.051 dB	0.057 dB	0.064 dB	0.071 dB	0.078 dB	0.088 dB
(75 to 100) GHz	0.038 dB	0.041 dB	0.044 dB	0.046 dB	0.053 dB	0.06 dB	0.067 dB	0.074 dB	0.084 dB
(100 to 110) GHz	0.044 dB	0.048 dB	0.051 dB	0.054 dB	0.061 dB	0.068 dB	0.075 dB	0.082 dB	0.098 dB
(110 to 120) GHz	0.44 dB	0.44 dB	0.44 dB	0.44 dB	0.45 dB	0.45 dB	0.46 dB	0.47 dB	0.48 dB

**Electrical - RF Microwave**

El Segundo, CA

Parameter/Equipment		Transmission S12/S21 - Phase							
Reference Standard, Method, and/or Equipment		Comparison to Keysight network analyzer							
Expanded Uncertainty of Measurement (+/-)									
Range	(0 to 3) dB	(3 to 6) dB	(6 to 10) dB	(10 to 20) dB	(20 to 30) dB	(30 to 40) dB	(40 to 50) dB	(50 to 60) dB	(60 to 70) dB
DC to 10 MHz	0.004 3°	0.039°	0.048°	0.061°	0.084°	0.006 2°	0.007 9°	0.008 2°	0.008 5°
10 MHz to 2 GHz	0.002 9°	0.035°	0.04°	0.048°	0.067°	0.0062°	0.007 8°	0.007 9°	0.008 1°
(2 to 8) GHz	0.002 9°	0.035°	0.0°	0.048°	0.067°	0.006 8°	0.008 2°	0.008 4°	0.008 5°
(8 to 20) GHz	0.032°	0.035°	0.04°	0.048°	0.067°	0.00 91°	0.01°	0.01°	0.01°
(20 to 26.5) GHz	0.15°	0.15°	0.15°	0.15°	0.16°	0.011°	0.012°	0.012°	0.012°

**Electrical - RF Microwave**

El Segundo, CA

Parameter/Equipment		Transmission S12/S21 - Phase							
Reference Standard, Method, and/or Equipment		Comparison to Keysight network analyzer							
<b>Expanded Uncertainty of Measurement (+/-)</b>									
Range	(0 to 3) dB	(3 to 6) dB	(6 to 10) dB	(10 to 20) dB	(20 to 30) dB	(30 to 40) dB	(40 to 50) dB	(50 to 60) dB	(60 to 70) dB
(26.5 to 33) GHz	0.18°	0.18°	0.19°	0.19°	0.19°	0.015°	0.016°	0.016°	0.016°
(33 to 40) GHz	0.23°	0.24°	0.24°	0.24°	0.24°	0.25°	0.26°	0.28°	0.4°
(40 to 45) GHz	0.29°	0.29°	0.29°	0.29°	0.3°	0.31°	0.32°	0.35°	0.56°
(45 to 50) GHz	0.31°	0.31°	0.31°	0.31°	0.32°	0.32°	0.33°	0.37°	0.57°
(50 to 60) GHz	0.28°	0.38°	0.38°	0.38°	0.38°	0.39°	0.4°	0.43°	0.65°
(60 to 67) GHz	0.28°	0.43°	0.43°	0.43°	0.44°	0.44°	0.45°	0.49°	0.73°
(50 to 75) GHz	0.28°	0.3°	0.32°	0.34°	0.38°	0.42°	0.47°	0.52°	0.58°
(75 to 100) GHz	0.25°	0.27°	0.29°	0.31°	0.35°	0.4°	0.44°	0.49°	0.56°
(100 to 110) GHz	0.29°	0.32°	0.34°	0.36	0.4°	0.45°	0.49°	0.55°	0.65°
(110 to 120) GHz	3°	3°	3°	3°	3°	3.1°	3.1°	3.2°	3.3°

**Length – Dimensional Metrology**

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Calipers <sup>3</sup>	(0 to 12) in (>12 to 60) in	(310 + 2L) μin (310 + 4L) μin	Comparison to gage blocks
Connector Gage Masters Flatness Step	to 0.001 in 0 to 0.35 in	25 μin 150 μin	Comparison to an optical flat electronic indicator
Cylindrical Plug Gages <sup>3</sup>	to 4 in	(20 + 10D) μin	Comparison to gage blocks
Cylindrical Ring Gages <sup>3</sup>	to 6 in	(6 + 12L) μin	Comparison to gage blocks
Dial and Digital Indicators			
Digital Indicators	(0 to 1) in (1 to 2) in (2 to 6) in	35 μin 38 μin 80 μin	Comparison to gage blocks
Dial Indicators	(0 to 1) in (1 to 6) in	64 μin 621 μin	

**Length – Dimensional Metrology**

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Electronic Gage Amplifiers	(>0 to 0.1) in	10 μin	Comparison to gage blocks
Gage Blocks <sup>3</sup>	(0.01 to 4) in Length Parallelism/VIL	(2 + 1L) μin 1.2 μin	Electromechanical comparison
Height Gages <sup>3</sup>	(>0 to 48) in	(310 + 4L) μin	Comparison to gage blocks
Length – Non-Contact Measurement <sup>3</sup>	(>0 to 12) in (12 to 60) in	(10 + 10L) μin (100 + 5L) μin	Comparison to laser interferometer
Outside Micrometer Length <sup>3</sup>	(0 to 12) in (>12 to 48) in	(30 + 6L) μin (30 + 7L) μin	Comparison to gage blocks
Outside Micrometer Anvil Flatness	(>0 to 48) μin	6 μin	Comparison to optical flats
Inside Micrometer Length <sup>3</sup>	(>0 to 12) in	(30 + 6L) μin	Comparison to gage blocks
Depth Micrometer Length <sup>3</sup>	(>0 to 12) in	(30 + 6L) μin	Comparison to gage blocks
Thread Measuring Wires	(4 to 80) TPI	17 μin	Mechanical comparison
Torque Moment Arms and Wheels <sup>3</sup>	Up to 48 in	(150 + 50L) μin	Comparison to gage blocks, electronic amplifier
Alignment Collimator	(-30 to 30) arc s 2 ft to Infinity Focus	1 arc s	Comparison to optical wedge
Autocollimators	(>0 to 1 800) arc s	0.15 % of reading + 0.3 arc s	Comparison to laser interferometer
Angle Generator	(0.05 to 100) arc s (100 to 180) arc s (180 to 1 000) arc s	0.4 arc s 0.6 arc s 0.33% of reading	Comparison to laser interferometer
Angle Gage Blocks	1 arcsec to 45 °	1.1 arc s	Comparison to angle blocks; autocollimator
Electronic Levels	(>0 to 200) arc s (200 to 1 000) arc s	0.8 arc s 2.9 arc s	Comparison to laser interferometer
Bubble Levels <sup>3</sup>	(>0 to 15) in	0.65R μin	Comparison to gage blocks

**Length – Dimensional Metrology**

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Sine Bars & Plates Angle Parallelism	(>0 to 45) ° 0.10 in	2.4 arc s 33 μin	Comparison to angle gage blocks, gaging amplifier
Squares and Angle Plates	90 °	6.5 arc s	Comparison to cylindrical square
Protractor	(>0 to 90) °	53 arc s	Comparison to sine bar, gage blocks, precision level
Optical Flat Flatness Parallelism	Up to 4 in	4 μin 1.2 μin	Comparison to optical flats, gage block comparator
Optical Wedge	Up to 30 arc s	0.3 arc s	Comparison to laser interferometer
Theodolite/Transmit/ Alignment Telescope Collimation Line of Sight Trunnion Axis	Infinity focus 2 ft to infinity focus (60 to 135) °	1.1 arc s 1.6 arc s 1.2 arc s	Comparison to alignment collimator
V-Blocks Parallelism	to 6 in	37 μin	Comparison to Gaging amplifier
Perpendicularity	to 6 in	6.5 arc s	Cylindrical square
Surface Plate <sup>3</sup> Overall Flatness Local Area Flatness	(60 x 96) in	12 √D μin 30 μin	Comparison to electronic level repeat reading gage
Thread Plug Gages Pitch Diameter Major Diameter	to 1 in	60 μin 50 μin	Comparison to 3 wire method Gage blocks
Thread Ring Gages Pitch Diameter	to 1 in	160 μin	Comparison to thread setting plug

**Mass and Mass Related**

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Gas Flow	10 sccm to 30 slpm (30 to 100) slpm	0.5 % of reading 0.75 % of reading	Comparison to mass flow standards

**Mass and Mass Related**

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Helium Leak Rate	(10 <sup>-09</sup> to 10 <sup>-03</sup> ) sccs	11 % of reading	Comparison to standard leak
Force	(>0 to 50 000) lbf (50 000 to 100 000) lbf	0.05 % of reading 0.22 % of reading	Comparison to deadweight, load cell
Mass Standards	(1 to 500) mg 500 mg to 2 g (2 to 5) g (5 to 10) g (10 to 20) g (20 to 50) g (50 to 100) g (100 to 200) g (200 to 500) g 500 g to 1 kg (1 to 2) kg (2 to 5) kg 10 kg  1 lb 2 lb 5 lb 10 lb 20 lb 25 lb 50 lb	0.012 mg 0.043 mg 0.046 mg 0.075 mg 0.12 mg 0.23 mg 0.46 mg 0.91 mg 2.3 mg 5.2 mg 26 mg 33 mg 0.25 g  7.3 E-6 lb 1.5 E-5 lb 5.7 E-5 lb 8.5 E-5 lb 5.6E-4 lb 5.7 E-4 lb 6.6 E-4 lb	Comparison to reference weights, electronic balances
Pressure	(0.2 to 100) psia (100 to 1 000) psia (1 000 to 15 000) psig (15 000 to 20 000) psig	0.003 6% of reading 0.004% of reading 0.004 4% of reading 0.006 2% of reading	Comparison to deadweight tester
Scales and Balances <sup>4</sup>	(5 to 500) mg (0.5 to 5) g (5 to 10) g (10 to 20) g (20 to 50) g (50 to 100) g (100 to 200) g (200 to 500) g (500 to 1000) g (1 to 2) kg (2 to 5) kg (5 to 20) kg (20 to 32) kg	0.012 mg 0.044 mg 0.064 mg 0.093 mg 0.14 mg 0.3 mg 0.6 mg 1.5 mg 3 mg 6.6 mg 16 mg 0.1 g 0.13 g	Comparison to reference weights

**Mass and Mass Related**

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Scales and Balances <sup>4</sup>	(50 to 2 000) lb (2 000 to 5 000) lb	0.025 % of reading 0.06 % of reading	Comparison to reference weights
Vacuum Ionization Gages, Inverted Magnetron Gages, Cold Cathode Gages, Residual Drag Gages	2.0 x 10 <sup>-7</sup> torr 5.0 x 10 <sup>-7</sup> torr 9.0 x 10 <sup>-7</sup> torr	24 % of reading 21 % of reading 11 % of reading	Comparison to ionization gage
Vacuum Ionization Gages, Inverted Magnetron Gages, Cold Cathode Gages, Residual Drag Gages	2.0 x 10 <sup>-6</sup> torr 5.0 x 10 <sup>-6</sup> torr 9.0 x 10 <sup>-6</sup> torr 2.0 x 10 <sup>-5</sup> torr 5.0 x 10 <sup>-5</sup> torr 9.0 x 10 <sup>-5</sup> torr 2.0 x 10 <sup>-4</sup> torr 5.0 x 10 <sup>-4</sup> torr 9.0 x 10 <sup>-4</sup> torr	6.7 % of reading 12 % of reading 4.7 % of reading 6.7 % of reading 4.9 % of reading 4 % of reading 6.4 % of reading 4.4 % of reading 3.2 % of reading	Comparison to spinning rotor gage
Thermocouple Vacuum Gage/Capacitance Manometer	(0.01 to 0.1) torr (0.1 to 10) torr (10 to 1 000) torr	0.6 % of reading + 0.2 mtorr 0.6 % of reading + 1 mtorr 0.006 6 % of reading	Capacitance diaphragm comparison to deadweight tester
Torque Transducers	10 ozf in to 2 000 lbf ft	0.03% of reading	Comparison to standard weights, torque moment Arms
Torque Wrench and Torque Screwdriver	5 ozf in to 2 000 lbf ft	0.7% of reading	Comparison to torque testers

**Photometry and Radiometry**

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Fiber Optic Attenuation Single Mode	(1 310, 1 550) nm (0 to 60) dB	0.021 dB	Comparison to optical power meter
Multi-Mode	(850, 1 300) nm (0 to 60) dB	0.021 dB	

**Photometry and Radiometry**

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Fiber Optic Power Single Mode	(1 310, 1 550) nm (-60 to 5) dBm	0.047 dB	Comparison to optical power meter
Multi-Mode	(850, 1 300) nm (-60 to 5) dBm	0.047 dB	
Fiber Optic Wavelength Wavelength Meter	(1 528 to 1 563) nm	0.001 4 nm	Comparison to NIST SRM 2519
Fiber Optic Wavelength Measure (Single Mode)	(700 to 1 700) nm	2 pm	Comparison to wavelength meter
Fiber Optic Wavelength Measure (Multi Mode)	(550 to 2 000) nm	2.9 nm	Comparison of a monochromator
Luminous Intensity	(20 to 500) fc	0.8% of reading	Comparison to NIST luminous intensity lamp

**Thermodynamic**

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Dewpoint / Frostpoint Indicators	(-80 to 10) °C	0.35 °C	Comparison to a humidity generator
Relative Humidity	(10 to 90) %RH	0.8 %RH	Comparison to a humidity generator
Infrared Thermometers	(-15 to 0) °C (0 to 100) °C (100 to 200) °C (200 to 350) °C (350 to 500) °C	1.3 °C 1.2 °C 1.4 °C 1.9 °C 2.4 °C	Comparison to infrared calibrator $\epsilon = 0.95, \lambda = (8 \text{ to } 14) \mu\text{m}$
Resistance Thermometry Fixed Point	-195.5 °C	0.002 3 °C	Comparison to DCC Resistance Bridge, NIST SPRT comparator
Resistance Thermometry Fixed Point	-38.8344 °C	0.001 4 °C	Comparison to DCC Resistance Bridge, NIST SPRT, TP Mercury cell
Resistance Thermometry Fixed Point	0.01 °C	0.000 4 °C	Comparison to DCC Resistance Bridge, NIST SPRT, TP Water cell



ANSI National Accreditation Board

Thermodynamic

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Resistance Thermometry Fixed Point	231.9280 °C	0.002 5 °C	Comparison to DCC Resistance Bridge, NIST SPRT, FP Tin cell
Resistance Thermometry Fixed Point	419.527 °C	0.002 8 °C	Comparison to DCC Resistance Bridge, NIST SPRT, FP Zinc cell
Temperature	(-80 to 0) °C (1 to 125) °C (126 to 300) °C (301 to 1 000) °C	0.005 °C 0.003 °C 0.005 °C 0.3 °C	Comparison to super thermometer, SPRT, TPW cell, thermocouple
Optical Pyrometer	(800 to 849) °C (850 to 949) °C (950 to 1 049) °C (1 050 to 1 149) °C (1 150 to 1 249) °C (1 250 to 1 349) °C (1 350 to 1 549) °C (1 550 to 1 649) °C (1 650 to 1 749) °C (1 750 to 1 849) °C (1 850 to 1 949) °C (1 950 to 2 049) °C (2 050 to 2 149) °C (2 150 to 2 249) °C (2 250 to 2 300) °C	3.3 °C 3 °C 2.6 °C 3.1 °C 2.4 °C 2.5 °C 2.8 °C 3.1 °C 2.9 °C 3.1 °C 3.2 °C 4.1 °C 5 °C 4.5 °C 3.8 °C	Comparison to NIST Tungsten strip lamp
Temperature – Source (stimulation)	(-210 to -200) °C (-200 to 0) °C (0 to 100) °C (100 to 300) °C (300 to 400) °C (400 to 630) °C (630 to 760) °C (760 to 800) °C (800 to 1 200) °C (1 200 to 1 372) °C	0.22 °C 0.039 °C 0.055 °C 0.070 °C 0.078 °C 0.093 °C 0.14 °C 0.18 °C 0.19 °C 0.32 °C	Comparison to a resistance, voltage generator

**Time and Frequency**

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Allan Variance	(1, 5, 10) MHz	$7.8 \times 10^{-14}$ Hz	Comparison to phase noise test set
Frequency - Measure	(1, 5, 10) MHz	5.8 parts in $10^{14}$ Hz	Comparison to NIST TMAS System
Frequency – Source	10 MHz	510 pHz/Hz	Comparison to Rubidium frequency standard
Frequency – Source	(0.1 to 1) Hz 1 Hz to 250 kHz 250 kHz to 1 MHz 1 MHz to 12.4 GHz (12.4 to 46) GHz	2.0 $\mu$ Hz/Hz + 0.4 $\mu$ Hz 2.4 $\mu$ Hz/Hz 5.1 nHz/Hz + 0.13 mHz 5.2 nHz/Hz 5.2 nHz/Hz + 2 $\mu$ Hz	Comparison to Rubidium frequency standard and a function generator
Frequency – Measure	(0.1 to 1) Hz (1 to 10) Hz (10 to 100) Hz 100 Hz to 1 kHz (1 to 100) kHz 100 kHz to 10 MHz 10 MHz to 12.4 GHz (12.4 to 46) GHz	1.2 pHz/Hz + 63 pHz 0.61 pHz/Hz + 0.85 pHz 4.5 pHz/Hz + 4.1 nHz 23 pHz/Hz + 22 pHz 23 pHz/Hz + 0.13 nH 23 pHz/Hz + 33 nHz 23 pHz/Hz + 32 nHz 24 pHz/Hz + 1.1 Hz	Comparison to frequency counter
Stop Watches, Timers	24 hr	0.23 s/24 hr	Comparison to NIST TMAS System
Time Interval – Measure	(10 to 430) ps 430 ps to 1 $\mu$ s 1 $\mu$ s to 50 ms 50 ms to 1 s (1 to 10) s (10 to 100) s	12 ms/s + 1.2 ps 6.7 ps 36 ns/s + 7.5 ps 1.9 ns 26 ps/s + 2.1 ns 33 ps/s + 2.7 ns	Comparison to a frequency counter and an oscilloscope
Transition - Measure	(8 to 30) ps (30 to 50) ps (50 to 200) ps (200 to 500) ps	1.2 ps 1.3 ps 10 fs/s + 0.9 ps 9.4 fs/s + 1 ps	Comparison to an oscilloscope


**Time and Frequency**

El Segundo, CA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Jitter - Source	(0.01 to 25) ps 2 GHz 2.5 GHz 2.75 GHz 3 GHz 3.2 GHz 5 GHz 8 GHz 10 GHz 12 GHz 13 GHz 14 GHz 15 GHz 28 GHz 32 GHz	0.12 ps 44 fs 65 fs 0.13 ps 0.13 ps 0.1 ps 52 fs 31 fs 50 fs 50 fs 0.1 ps 50 fs 42 fs 37 fs	Comparison to a signal generator
Jitter - Measure	(0.1 to 130) ps 200 kHz to 15 GHz	1.9 ps	Comparison to an oscilloscope

[Return to Site listing \(top\)](#)

[Go to Notes \(bottom\)](#)

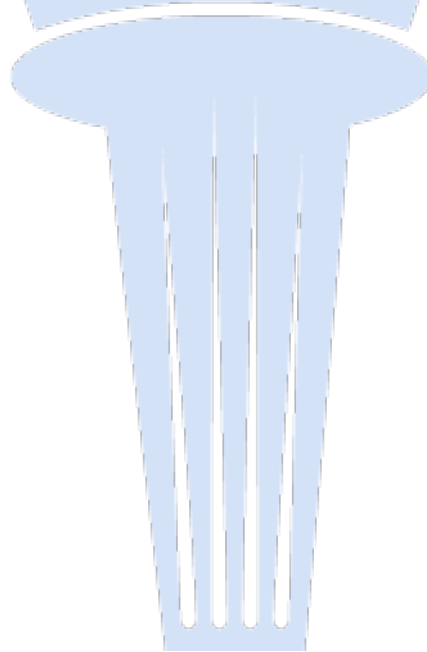



ANSI National Accreditation Board

**Services performed at satellite laboratory**

1346 Yellowwood Road  
Kimballton, IA 51543

Nate Potts 712-248-6069  
[nate.potts@keysight.com](mailto:nate.potts@keysight.com) [www.keysight.com](http://www.keysight.com)

Electrical – RF/Microwave

Kimballton, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
ISN –			
Phase	(0 to 360)°	3°	CISPR 22, CISPR 32, CISPR 16-1-2 E5061B, E5071C Network Analyzers
Insertion Loss	150 kHz to 80 MHz (0 to 110) dB	0.36 dB	
Impedance	150 kHz to 80 MHz (0 to 5000) Ω	2.4 Ω	
Longitudinal Conversion Loss	150 kHz to 80 MHz (0 to 110) dB	0.88 dB	
Decoupling Attenuation	150 kHz to 80 MHz (0 to 110) dB	0.36 dB	
LISN			
Insertion Loss	(0 to 110) dB		
	9 kHz to 108 MHz	0.66 dB	
	(108 to 400) MHz	0.86 dB	
	(0 to 110) dB		
	150 kHz to 100 MHz	0.38 dB	
	(100 to 200) MHz	0.61 dB	
	(200 to 400) MHz	1.4 dB	
	(400 to 600) MHz	1.3 dB	
	(600 to 800) MHz	1.4 dB	
	800 MHz to 1 GHz	2.3 dB	
Impedance – Magnitude	(0 to 5 000) Ω		
	9 kHz to 100 MHz	0.2 Ω	
	(100 to 200) MHz	0.7 Ω	
	(200 to 400) MHz	1.2 Ω	

**Electrical – RF/Microwave**

Kimballton, IA

<b>Parameter/Equipment</b>	<b>Range</b>	<b>Expanded Uncertainty of Measurement (+/-)</b>	<b>Reference Standard, Method, and/or Equipment</b>
LISN Impedance – Magnitude	(0 to 5 000) $\Omega$ 150 kHz to 100 MHz	0.35 $\Omega$	ANSI C63.4, CISPR 25 & CISPR 16-1-2, ISO 7637-2, MIL-STD-461, RTCA DO-160
	(100 to 200) MHz	1.3 $\Omega$	
	(200 to 400) MHz	2.3 $\Omega$	
	(400 to 600) MHz	2.2 $\Omega$	
	(600 to 800) MHz	1.9 $\Omega$	
	800 MHz to 1 GHz	2.2 $\Omega$	
Impedance – Phase	(0 to 360) $^{\circ}$ 9 kHz to 100 MHz	3.6 $^{\circ}$	
	(100 to 200) MHz	3.4 $^{\circ}$	
	(200 to 400) MHz	3.2 $^{\circ}$	
Isolation	(0 to 110) dB 9 kHz to 100 MHz	0.36 dB	
	(100 to 200) MHz	1.1 dB	
	(200 to 400) MHz	1.6 dB	
	400 MHz to 1.0 GHz	1.6 dB	
Current Probes & Bulk Current Injection Probes Insertion Loss	(0 to 110) dB 5 Hz to 500 MHz	0.77 dB	CISPR 16-1-2, IEC/EN 61000-4-6 E5061B, E5071C Network Analyzers, BNC & Type “N” calibration standards
	500 MHz to 2.4 GHz	1.1 dB	
Transfer Impedance	(0 to 110) dB 5 Hz to 500 MHz	0.77 dB	
	500 MHz to 2.4 GHz	1.1 dB	
CDN’s & Adapters (50 to 150) $\Omega$ Adapter Insertion Loss	(0 to 110) dB 10 kHz to 230 MHz	1.2 dB	IEC/EN 61000-4-6 CISPR 16-1-2 E5061B, E5071C Network Analyzers, BNC and Type “N” calibration standards
Coupling Factor	(0 to 110) dB 10 kHz to 230 MHz	1.1 dB	
Impedance	(0 to 5000) $\Omega$ 10 kHz to 230 MHz	3.5 $\Omega$	
CDN’s & Adapters – (50 to 150) $\Omega$ Voltage Division Factor	(0 to 110) dB 10 kHz to 230 MHz	0.25 dB	IEC/EN 61000-4-6 CISPR 16-1-2 Agilent E5061B ENA Network Analyzer

**Electrical – RF/Microwave**

Kimballton, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Absorbing Clamps	(0 to 110) dB 30 MHz to 1 GHz 30 MHz to 1 GHz	0.32 dB 2.4 dB	CISPR 16-1-3 Annex B, Agilent E5061B Network Analyzer, original calibration method, OATS/CALTS CISPR 16-1-3 Annex C, Agilent E5061B
Injection Clamps	(0 to 110) dB (0.01 to 1) MHz (1 to 1 000) MHz	0.3 dB 0.35 dB	IEC/EN 61000-4-6 E5061B
NSA/CALTS Measurements	(0 to 110) dB (30 to 1 000) MHz	0.1 dB	ANSI C63.5, ANSI C63.4, EN 50147-2 (1997) CISPR 16-1-4, CISPR 16-1-5 Agilent E5061B & E5071C HP 8753D, Agilent E8364C, Keysight N5225A Network Analyzers
Site VSWR Measurements	(0 to 110) dB (1 to 3) GHz (3 to 18) GHz	0.66 dB 0.84 dB	CISPR 16-1-4, CISPR 16-1-5 Agilent E8364C, Keysight N5225A Network Analyzers
Field Uniformity	(0 to 110) dB 26 MHz to 18 GHz	1.2 dB	IEC/EN 61000-4-3
ESD Targets Frequency Response	(0 to 110) dB DC to 4 GHz	0.26 dB	IEC 61000-4-2, ISO 10605 Agilent ENA E5071C Network Analyzer, Fluke 123 Scopemeter, HP 3478A Multimeter, Solar 7144-1.0 Decade Resistor
Low Frequency Transfer Function	(0 to 30) A	0.32 % of reading	
Insertion Loss	(0 to 110) dB Up to 300 kHz (0.30 to 10) MHz (0.010 to 3.0) GHz (3.0 to 4.0) GHz	0.072 dB 0.076 dB 0.08 dB 0.092 dB	

**Electrical – RF/Microwave**

Kimballton, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
ESD Simulators –			
Contact Voltage (Positive & Negative)	(0 to 2) kV (2 to 8) kV (8 to 15) kV (15 to 30) kV (30 to 40) kV	2.6 % of reading 0.7 % of reading 0.6 % of reading 0.54 % of reading 0.72 % of reading	IEC/EN 61000-4-2; ISO 10605; SAE J1113-13, GR1089 TEK TDS 7404 Oscilloscope IEC ESD target applied kilovolt 149-3 High Voltage Meter
Rise Time	(0 to 2) ns	61 ps	
Peak Current	(0 to 40) A	5 % of reading	
30 ns Current	(0 to 40) A	5.6 % of reading	
60 ns Current	(0 to 40) A	6.1 % of reading	
Air Discharge Voltage (Positive & Negative)	(0 to 2) kV (2 to 20) kV (20 to 40) kV	0.15 % of reading 0.61 % of reading 1.2 % of reading	
Rise Time – RC Time Constant  (at ± 15 kV) 330 pF probe 150 pF probe	(0 to 2) ns  600 ns ± 130 ns 300 ns ± 60 ns	61 ps  7.2 ns 6 ns	
Magnetic Field Strength Meters –			Comparison to Reference Magnets, Standard Field using Helmholtz coil
DC	(50 to 2 000) G	2 % of reading	
AC	0.20 mG to 20 G	0.33 % +1.2 mG	
RF Pre-Amplifiers, Amplifiers – Gain	(0 to 110) dB 5 Hz to 18 GHz (18 to 50) GHz	0.97 dB 1 dB	IEEE 291 Agilent E5061B, E5071C Agilent E8364C, Keysight N5225A Network Analyzer
RF Isotropic E-Field Probe	(0 to 15) dB 5 kHz to 800 MHz		IEEE 1309, IEC/EN 61000-4-3 Substitution, Calculated using TEM Cell
Field Strengths up to 1200 V/m	Frequency Response	0.73 dB	
	Linearity	0.91 dB	
	Isotropic Response	0.92 dB	

**Electrical – RF/Microwave**

Kimballton, IA

<b>Parameter/Equipment</b>	<b>Range</b>	<b>Expanded Uncertainty of Measurement (+/-)</b>	<b>Reference Standard, Method, and/or Equipment</b>
RF Isotropic E-Field Probe  Field Strengths up to 1200 V/m	(0 to 15) dB 10 kHz to 1 000 MHz Frequency Response Linearity Isotropic Response	0.86 dB 1.1 dB 1.2 dB	IEEE 1309, IEC/EN 61000-4-3 Substitution, Calculated Tri-plate
RF Isotropic E-Field Probe  Field Strengths up to 1200 V/m	(0 to 15) dB 10 kHz to 1 000 MHz Frequency Response Linearity Isotropic Response	0.79 dB 0.94 dB 0.97 dB	IEEE 1309, IEC/EN 61000-4-3 Substitution using GTEM Cell
RF Isotropic E-Field Probe  Field Strengths up to 1200 V/m	(0 to 15) dB 450 MHz to 18 GHz Frequency Response Linearity Isotropic Response 18 to 40 GHz Frequency Response Linearity Isotropic Response	0.91 dB 1.1 dB 1.1 dB 1.1 dB 1.7 dB 1.7 dB	IEEE 1309, IEC/EN 61000-4-3 Substitution, Calculated using Anechoic chamber
RF Isotropic E-Field Probe  Field Strengths up to 1200 V/m	(0 to 15) dB 40 to 60 GHz Frequency Response Linearity Isotropic Response	1.7 dB 0.54 dB 0.47 dB	IEEE 1309, IEC/EN 61000-4-3 Substitution using Anechoic chamber
Electronic E-Field Probes	(0 to 15) dB 10 kHz to 5 GHz Frequency Response Linearity Channel Match Factor	1.3 dB 0.83 dB 1 dB	IEEE 1309, IEC/EN 61000-4-3 Substitution using FP 5000 type probe
Electronic E-Field Probes	(0 to 15) dB 10 kHz to 5 GHz Isotropic Response	0.83 dB	IEEE 1309, IEC/EN 61000-4-3 FP 5000 type probe
Electronic E-Field Probes	(0 to 15) dB 80 MHz to 18 GHz Frequency Response Linearity	1.9 dB 0.84 dB	IEEE 1309, IEC/EN 61000-4-3 Substitution, Calculated using FP 2080 type probe
Electronic E-Field Probes	(0 to 15) dB (18 to 40) GHz Frequency Response Linearity	2.3 dB 1.3 dB	IEEE 1309, IEC/EN 61000-4-3 Substitution using FP 2080 type probe

**Electrical – RF/Microwave**

Kimballton, IA

<b>Parameter/Equipment</b>	<b>Range</b>	<b>Expanded Uncertainty of Measurement (+/-)</b>	<b>Reference Standard, Method, and/or Equipment</b>
Electronic E-Field Probes	(0 to 5) dB 80 MHz to 40 GHz Isotropic Response	1.2 dB	IEEE 1309, IEC/EN 61000-4-3 FP 2080 type probe
Electronic E-Field Probes	(0 to 5) dB 80 MHz to 18 GHz Channel Match Factor	1 dB	IEEE 1309, IEC/EN 61000-4-3 Substitution, Calculated using FP 2080 type probe
Electronic E-Field Probes	(0 to 5) dB (18 to 40) GHz Channel Match Factor	1.3 dB	IEEE 1309, IEC/EN 61000-4-3 Substitution using FP 2080 type probe
Dipole Antennae 3 meter distance	(0 to 110) dB (30 to 60) MHz (50 to 150) MHz (140 to 400) MHz (400 to 1 000) MHz	0.5 dB 0.48 dB 0.55 dB 0.6 dB	Calibration Test Site (CALTS) / Open Area Test Site (OATS), Keysight E5071C, N5225A, E8364B Network Analyzers ANSI C63.5, CISPR 16-1-6: Standard Site Method, Horizontal/ Vertical Polarization
Dipole Antennae 3 meter distance	(0 to 110) dB (30 to 60) MHz (50 to 150) MHz (140 to 400) MHz (400 to 1 000) MHz	0.52 dB 0.55 dB 0.60 dB 0.62 dB	Calibration Test Site (CALTS) / Open Area Test Site (OATS), Keysight E5071C, N5225A, E8364B Network Analyzers ANSI C63.5, CISPR 16-1-6: Reference Antenna Method, Horizontal/ Vertical Polarization
Dipole Antennae 3 meter distance	(0 to 110) dB (30 to 60) MHz (50 to 150) MHz (140 to 400) MHz (400 to 1 000) MHz	0.45 dB 0.52 dB 0.45 dB 0.58 dB	Calibration Test Site (CALTS) / Open Area Test Site (OATS), Keysight E5071C, N5225A, E8364B Network Analyzers ANSI C63.5, CISPR 16-1-6, SAE ARP: Identical Antenna Method, Horizontal/Vertical Polarization

Electrical – RF/Microwave

Kimballton, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Dipole Antennae 3 meter distance	(0 to 110) dB (30 to 1 000) MHz	0.59 dB	Calibration Test Site (CALTS) / Open Area Test Site (OATS), Keysight E5071C, N5225A, E8364B Network Analyzers ANSI C63.5, CISPR 16-1-6: Standard Antenna Method, Horizontal/Vertical Polarization
Dipole Antennae 3 meter distance	(0 to 110) dB (30 to 1 000) MHz	0.4 dB	Calibration Test Site (CALTS) / Open Area Test Site (OATS), Keysight E5071C, N5225A, E8364B Network Analyzers ANSI C63.5, CISPR 16-1-6: Three Antenna Method, Horizontal/Vertical Polarization
Dipole Antennae 10 meter distance	(0 to 110) dB (30 to 60) MHz (50 to 150) MHz (140 to 400) MHz (400 to 1 000) MHz	0.41 dB 0.45 dB 0.51 dB 0.55 dB	Calibration Test Site (CALTS) / Open Area Test Site (OATS), Keysight E5071C, N5225A, E8364B Network Analyzers ANSI C63.5, CISPR 16-1-6: Standard Site Method, Horizontal/Vertical Polarization
Dipole Antennae 10 meter distance	(0 to 110) dB (30 to 60) MHz (50 to 150) MHz (140 to 400) MHz (400 to 1 000) MHz	0.35 dB 0.4 dB 0.45 dB 0.51 dB	Calibration Test Site (CALTS) / Open Area Test Site (OATS), Keysight E5071C, N5225A, E8364B Network Analyzers ANSI C63.5, CISPR 16-1-6: Reference Antenna Method, Horizontal/Vertical Polarization

**Electrical – RF/Microwave**

Kimballton, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Dipole Antennae 10 meter distance	(0 to 110) dB (30 to 60) MHz (50 to 150) MHz (140 to 400) MHz (400 to 1 000) MHz	0.41 dB 0.38 dB 0.45 dB 0.5 dB	Calibration Test Site (CALTS) / Open Area Test Site (OATS), Keysight E5071C, N5225A, E8364B Network Analyzers ANSI C63.5, CISPR 16-1-6: Identical Antenna Method, Horizontal/Vertical Polarization
Dipole Antennae 10 meter distance	(0 to 110) dB (30 to 1 000) MHz	0.63 dB	Calibration Test Site (CALTS) / Open Area Test Site (OATS), Keysight E5071C, N5225A, E8364B Network Analyzers ANSI C63.5, CISPR 16-1-6: Standard Antenna Method, Horizontal/ Vertical Polarization
Dipole Antennae 10 meter distance	(0 to 110) dB (30 to 1 000) MHz	0.41 dB	Calibration Test Site (CALTS) / Open Area Test Site (OATS), Keysight E5071C, N5225A, E8364B Network Analyzers ANSI C63.5, CISPR 16-1-6, SAE ARP 958: Three Antenna Method, Horizontal/ Vertical Polarization
Horn Antennae Log Periodic Antennas Dipole Antennas 1 meter distance	(0 to 110) dB 700 MHz to 50 GHz	0.45 dB	Fully Anechoic Room (FAR), Keysight N5225A, E8364B Network Analyzers SAE ARP 958: Identical
Horn Antennae Log Periodic Antennas Dipole Antennas 3 meter distance	(0 to 110) dB 700 MHz to 50 GHz	0.45 dB	Fully Anechoic Room (FAR), Keysight N5225A, E8364B Network Analyzers SAE ARP: Appendix C



ANSI National Accreditation Board

Electrical – RF/Microwave

Kimballton, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Horn Antennae Log Periodic Antennas Dipole Antennas 1 and 3 meter distance Far Field	(0 to 110) dB 700 MHz to 18 GHz (18 to 26.5) GHz (26.5 to 50) GHz	0.37 dB 0.42 dB 0.47 dB	Fully Anechoic Room (FAR), Keysight N5225A, E8364B Network Analyzers SAE ARP 958: Combo of Identical and Appendix C, Horizontal/Vertical Polarization
Horn Antennae Log Periodic Antennas Dipole Antennas 1 and 3 meter distance Far Field	(0 to 110) dB 700 MHz to 18 GHz (18 to 26.5) GHz (26.5 to 50) GHz (50 to 67) GHz	0.37 dB 0.42 dB 0.47 dB 0.21 dB	Fully Anechoic Room (FAR), Keysight N5225A, N5291A, E8364B Network Analyzers CISPR 16-1-6: Three Antenna Method, Horizontal/Vertical Polarization
Horn Antennae Log Periodic Antennas Dipole Antennas 1 and 3 meter distance Far Field	(0 to 110) dB 700 MHz to 18 GHz (18 to 26.5) GHz (26.5 to 50) GHz	0.37 dB 0.42 dB 0.47 dB	Fully Anechoic Room (FAR), Keysight N5225A, E8364B Network Analyzers ANSI C63.5: Standard Site Method, Horizontal/Vertical Polarization
Horn Antennae Log Periodic Antennas Dipole Antennas	(0 to 110) dB 700 MHz to 50 GHz Far Field Near Field	0.44 dB 0.5 dB	Fully Anechoic Room (FAR), Keysight N5225A, E8364B Network Analyzers ANSI C63.5: Identical Antenna Method, Three Antenna Method, Horizontal/Vertical Polarization

**Electrical – RF/Microwave**

Kimballton, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Horn Antennae Log Periodic Antennas Dipole Antennas	(0 to 110) dB 700 MHz to 50 GHz Time Domain	0.46 dB	Fully Anechoic Room (FAR), Keysight N5225A, E8364B Network Analyzers ANSI C63.5, CISPR 16-1-6: Identical Antenna Method, Three Antenna Method Horizontal/Vertical Polarization
Lens Antennas 1 and 3 meter distance Far Field	(1 to 110) dB (20 to 46) GHz	0.24 dB	Fully Anechoic Room (FAR), Keysight N5225A Network Analyzer CISPR 16-1-6: Three Antenna Method

**Electrical – RF/Microwave**

Kimballton, IA

Parameter/Equipment	Attenuation – Measure <sup>1</sup>											
Reference Standard, Method, and/or Equipment	Comparison to N5225A/C Network Analyzer and Calibration Kit											
Range	Expanded Uncertainty of Measurement (+/-)											
Frequency Ranges	Step Attenuation Level in dB											
	0	1	2	3	4	5	6	7	8	9	10	11
10 MHz ≤ f < 300 MHz	0.028	0.03	0.031	0.03	0.032	0.033	0.032	0.034	0.035	0.035	0.035	0.037
300 MHz ≤ f < 2 GHz	0.028	0.03	0.032	0.032	0.033	0.034	0.034	0.036	0.037	0.037	0.037	0.039
2 GHz ≤ f < 8 GHz	0.047	0.048	0.049	0.049	0.051	0.052	0.052	0.054	0.055	0.055	0.054	0.057
8 GHz ≤ f < 12 GHz	0.052	0.053	0.055	0.054	0.056	0.057	0.056	0.059	0.06	0.06	0.059	0.062
12 GHz ≤ f < 18 GHz	0.059	0.061	0.062	0.061	0.064	0.065	0.064	0.067	0.067	0.068	0.067	0.07
18 GHz ≤ f < 20 GHz	-	-	-	0.061	-	-	0.064	-	-	-	0.067	-
20 GHz ≤ f < 30 GHz	-	-	-	0.11	-	-	0.11	-	-	-	0.12	-
30 GHz ≤ f < 40 GHz	-	-	-	0.12	-	-	0.13	-	-	-	0.13	-

**Electrical – RF/Microwave**

Kimballton, IA

<b>Parameter/ Equipment</b>	Attenuation – Measure <sup>1</sup>											
<b>Reference Standard, Method, and/or Equipment</b>	Comparison to N5225A/C Network Analyzer and Calibration Kit											
<b>Range</b>	<b>Expanded Uncertainty of Measurement (+/-)</b>											
Frequency Ranges	Step Attenuation Level in dB											
	0	1	2	3	4	5	6	7	8	9	10	11
40 GHz ≤ f < 50 GHz	-	-	-	0.18	-	-	0.19	-	-	-	0.2	-

**Electrical – RF/Microwave**

Kimballton, IA

<b>Parameter/ Equipment</b>	Attenuation – Measure										
<b>Reference Standard, Method, and/or Equipment</b>	Comparison to N5225A/C Network Analyzer and Calibration Kit										
<b>Range</b>	<b>Expanded Uncertainty of Measurement (+/-)</b>										
Frequency Ranges	Step Attenuation Level in dB										
	20	30	40	50	60	70	80	90	100	110	
10 MHz ≤ f < 50 MHz	0.042	0.053	0.089	0.17	0.12	0.14	0.17	0.18	0.18	0.19	
50 MHz ≤ f < 500 MHz	0.042	0.053	0.063	0.095	0.097	0.11	0.12	0.14	0.14	0.16	
500 MHz ≤ f < 2 GHz	0.044	0.051	0.06	0.085	0.1	0.11	0.1	0.11	0.12	0.14	
2 GHz ≤ f < 8 GHz	0.061	0.051	0.078	0.11	0.14	0.19	0.15	0.2	0.2	0.25	
8 GHz ≤ f < 12 GHz	0.066	0.068	0.089	0.15	0.19	0.25	0.21	0.26	0.29	0.33	
12 GHz ≤ f < 18 GHz	0.074	0.074	0.096	0.16	0.34	0.39	0.35	0.4	0.41	0.47	
18 GHz ≤ f < 20 GHz	0.074	0.082	0.096	-	-	-	-	-	-	-	
20 GHz ≤ f < 26.5 GHz	0.12	0.12	0.12	-	-	-	-	-	-	-	
26.5 GHz ≤ f < 30 GHz	0.13	0.13	0.15	-	-	-	-	-	-	-	
30 GHz ≤ f < 40 GHz	0.14	0.15	0.17	-	-	-	-	-	-	-	
40 GHz ≤ f < 50 GHz	0.2	0.21	0.24	-	-	-	-	-	-	-	

**Electrical – RF/Microwave**

Kimballton, IA

Parameter/ Equipment		S11 - Reflection Magnitude								
Reference Standard, Method, and/or Equipment		Comparison to 85054B, 85031B, ET33700, 85056A, 85058B Calibration Kits								
Range	Expanded Uncertainty of Measurement (+/-)									
Frequency	Measured Magnitude (+/- Linear)									
	≤ 0.1	>0.1 to ≤ 0.2	>0.2 to ≤ 0.3	>0.3 to ≤ 0.4	>0.4 to ≤ 0.5	>0.5 to ≤ 0.6	>0.6 to ≤ 0.7	>0.7 to ≤ 0.8	>0.8 to ≤ 0.9	>0.9 to ≤ 1
5 Hz to 9 kHz	0.003 1	0.003 3	0.003 6	0.004 1	0.004 5	0.005 1	0.005 6	0.006 2	0.006 8	0.007 4
(9 to 100) kHz	0.003 1	0.003 3	0.003 6	0.004 1	0.004 5	0.005 1	0.005 6	0.006 2	0.006 8	0.007 4
(0.1 to 20 MHz	0.003 1	0.003 3	0.003 6	0.004 1	0.004 7	0.005 4	0.006 2	0.007 2	0.008	0.009 5
(0.02 to 2) GHz	0.000 54	0.000 62	0.000 7	0.000 81	0.000 93	0.001 1	0.001 2	0.001 4	0.001 6	0.001 7
(2 to 8) GHz	0.000 78	0.000 82	0.000 89	0.000 98	0.001 1	0.001 2	0.001 4	0.001 5	0.001 7	0.001 9
(8 to 20) GHz	0.001 4	0.001 4	0.001 5	0.001 5	0.001 6	0.001 7	0.001 8	0.002	0.002 3	0.002 6
(20 to 26.5) GHz	0.001 9	0.001 9	0.001 9	0.002	0.002	0.002 1	0.002 3	0.002 5	0.002 7	0.003 1
(26.5 to 40) GHz	0.003 9	0.004 1	0.004 4	0.004 9	0.005 6	0.006 6	0.007 7	0.009 1	0.011	0.012
(40 to 50) GHz	0.005 2	0.005 4	0.005 8	0.006 3	0.007	0.008 1	0.009 5	0.011	0.013	0.015
(50 to 67) GHz	0.014	0.014	0.014	0.014	0.014	0.014	0.015	0.015	0.015	0.016

**Electrical – RF/Microwave**

Kimballton, IA

Parameter/ Equipment		S11 - Reflection Phase								
Reference Standard, Method, and/or Equipment		Comparison to 85054B, 85031B, ET33700, 85056A, 85058B Calibration Kits								
Range	Expanded Uncertainty of Measurement (+/-)									
Frequency	Measured Magnitude (+/- Degrees)									
	≤ 0.1	>0.1 to ≤ 0.2	>0.2 to ≤ 0.3	>0.3 to ≤ 0.4	>0.4 to ≤ 0.5	>0.5 to ≤ 0.6	>0.6 to ≤ 0.7	>0.7 to ≤ 0.8	>0.8 to ≤ 0.9	>0.9 to ≤ 1
5 Hz to 9 kHz	1.9	1	0.77	0.65	0.58	0.53	0.50	0.48	0.47	0.47
(9 to 100) kHz	1.9	1	0.77	0.65	0.58	0.53	0.50	0.48	0.47	0.47

**Electrical – RF/Microwave**

Kimballton, IA

Parameter/ Equipment		S11 - Reflection Phase								
Reference Standard, Method, and/or Equipment		Comparison to 85054B, 85031B, ET33700, 85056A, 85058B Calibration Kits								
Range		Expanded Uncertainty of Measurement (+/-)								
Frequency	Measured Magnitude (+/- Degrees)									
	≤ 0.1	>0.1 to ≤ 0.2	>0.2 to ≤ 0.3	>0.3 to ≤ 0.4	>0.4 to ≤ 0.5	>0.5 to ≤ 0.6	>0.6 to ≤ 0.7	>0.7 to ≤ 0.8	>0.8 to ≤ 0.9	>0.9 to ≤ 1
(0.1 to 20 MHz)	1.9	1	0.78	0.67	0.61	0.59	0.58	0.58	0.6	0.6
(0.02 to 2) GHz	0.31	0.17	0.13	0.11	0.1	0.1	0.098	0.098	0.1	0.1
(2 to 8) GHz	0.45	0.24	0.17	0.14	0.12	0.12	0.11	0.11	0.11	0.11
(8 to 20) GHz	0.81	0.42	0.29	0.23	0.19	0.16	0.15	0.14	0.13	0.13
(20 to 26.5) GHz	1.1	0.55	0.38	0.29	0.24	0.2	0.18	0.17	0.17	0.17
(26.5 to 40) GHz	2.3	1.3	1	0.93	0.9	0.91	0.93	0.94	0.96	0.99
(40 to 50) GHz	3.1	1.7	1.3	1.2	1.1	1.1	1.1	1.2	1.2	1.2
(50 to 67 GHz)	8.1	4.1	2.7	2.0	1.6	1.4	1.2	1.1	1	0.95

**Electrical – RF/Microwave**

Kimballton, IA

Parameter/ Equipment		S21 - Transmission Magnitude								
Reference Standard, Method, and/or Equipment		Comparison to 85054B, 85031B, ET33700, 85056A, 85058B, 85059B Calibration Kits								
Range		Expanded Uncertainty of Measurement (+/-)								
Frequency	Measured Magnitude (dB)									
	10 to ≤ 0	>0 to ≤ 3	> 3 to ≤ 6	>-6 to ≤ 10	> 10 to ≤ 20	> 20 to ≤ 30	> 30 to ≤ 40	> 40 to ≤ 50	> 50 to ≤ 60	
5 Hz to 9 kHz	0.058	0.058	0.063	0.067	0.074	0.088	0.104	0.126	0.175	
(9 to 100) kHz	0.028	0.029	0.031	0.034	0.038	0.049	0.082	0.123	0.159	
(0.1 to 130) MHz	0.028	0.029	0.031	0.034	0.038	0.047	0.069	0.09	0.128	
(0.13 to 1.25) GHz	0.031	0.034	0.034	0.034	0.034	0.034	0.035	0.044	0.093	

**Electrical – RF/Microwave**

Kimballton, IA

Parameter/ Equipment		S21 - Transmission Magnitude							
Reference Standard, Method, and/or Equipment		Comparison to 85054B, 85031B, ET33700, 85056A, 85058B, 85059B Calibration Kits							
Range		Expanded Uncertainty of Measurement (+/-)							
Frequency	Measured Magnitude (dB)								
	10 to ≤ 0	>0 to ≤ 3	> 3 to ≤ 6	>-6 to ≤ 10	> 10 to ≤ 20	> 20 to ≤ 30	> 30 to ≤ 40	> 40 to ≤ 50	> 50 to ≤ 60
(1.25 to 4) GHz	0.031	0.034	0.034	0.034	0.034	0.034	0.034	0.035	0.044
(4 to 5) GHz	0.032	0.035	0.035	0.035	0.035	0.035	0.035	0.036	0.045
(5 to 26.5) GHz	0.034	0.036	0.036	0.036	0.036	0.036	0.037	0.037	0.038
(26.5 to 40) GHz	0.037	0.039	0.039	0.039	0.039	0.039	0.04	0.04	0.048
(40 to 50) GHz	0.04	0.043	0.043	0.043	0.043	0.043	0.043	0.044	0.051
(50 to 67) GHz	0.12	0.12	0.12	0.12	0.12	0.12	0.13	0.13	0.13

**Electrical – RF/Microwave**

Kimballton, IA

Parameter/ Equipment		S21 - Transmission Phase							
Reference Standard, Method, and/or Equipment		Comparison to 85054B, 85031B, ET33700, 85056A, 85058B Calibration Kits							
Range		Expanded Uncertainty of Measurement (+/-)							
Frequency	Measured Magnitude (+/- Degrees)								
	10 to ≤ 0	>0 to ≤ 3	> 3 to ≤ 6	> 6 to ≤ 0	> 10 to ≤ 20	> 20 to ≤ 30	> 30 to ≤ 40	> 40 to ≤ 50	> 50 to ≤ 60
5 Hz to 9 kHz	0.38	0.38	0.42	0.45	0.49	0.58	0.69	0.83	1.2
(9 to 100) kHz	0.19	0.19	0.21	0.22	0.25	0.32	0.54	0.82	1.1
(0.1 to 130) MHz	0.19	0.19	0.2	0.22	0.25	0.31	0.46	0.61	0.85
(0.13 to 1.25) GHz	0.37	0.37	0.37	0.37	0.38	0.38	0.38	0.41	0.68
(1.25 to 4) GHz	0.42	0.43	0.43	0.43	0.43	0.43	0.43	0.43	0.46
(4.0 to 5) GHz	0.5	0.5	0.5	0.5	0.5	0.5	0.5	0.5	0.53

**Electrical – RF/Microwave**

Kimballton, IA

<b>Parameter/Equipment</b>	S21 - Transmission Phase								
<b>Reference Standard, Method, and/or Equipment</b>	Comparison to 85054B, 85031B, ET33700, 85056A, 85058B Calibration Kits								
<b>Range</b>	<b>Expanded Uncertainty of Measurement (+/-)</b>								
<b>Frequency</b>	Measured Magnitude (+/- Degrees)								
	10 to ≤ 0	>0 to ≤ 3	> 3 to ≤ 6	> 6 to ≤ 0	> 10 to ≤ 20	> 20 to ≤ 30	> 30 to ≤ 40	> 40 to ≤ 50	> 50 to ≤ 60
(5 to 26.5) GHz	0.89	0.9	0.9	0.9	0.9	0.9	0.9	0.9	0.9
(26.5 to 40) GHz	1.2	1.2	1.2	1.2	1.2	1.2	1.2	1.2	1.2
(40 to 50) GHz	1.4	1.4	1.4	1.4	1.4	1.4	1.4	1.4	1.4
(50 to 67) GHz	0.79	0.79	0.79	0.79	0.8	0.81	0.83	0.86	0.89

**Electrical – RF/Microwave**

Kimballton, IA

<b>Parameter/Equipment</b>	Biconical Antennas		
<b>Reference Standard</b>	Calibration Test Site (CALTS) / Open Area Test Site (OATS), Keysight E5071C, N5225A, E8364B Network Analyzers		
<b>Method</b>	<b>Distance/Domain</b>	<b>Frequency Range</b>	<b>Expanded Uncertainty of Measurement (+/-)</b>
SAE ARP 958	1 Meter	(0 to 110) dB (20 to 70) MHz (70 to 200) MHz (200 to 300) MHz	0.33 dB 0.34 dB 0.37 dB
SAE ARP 958: Appendix C	3 Meter	(0 to 110) dB (20 to 70) MHz (70 to 200) MHz (200 to 300) MHz	0.37 dB 0.48 dB 0.37 dB
ANSI C63.5, CISPR 16-1-6: Standard Site Method, Horizontal/Vertical Polarization	3 Meter	(0 to 110) dB (20 to 70) MHz (70 to 200) MHz (200 to 300) MHz	0.93 dB 0.54 dB 0.25 dB

**Electrical – RF/Microwave**

Kimballton, IA

Parameter/Equipment	Biconical Antennas		
Reference Standard	Calibration Test Site (CALTS) / Open Area Test Site (OATS), Keysight E5071C, N5225A, E8364B Network Analyzers		
Method	Distance/ Domain	Frequency Range	Expanded Uncertainty of Measurement (+/-)
ANSI C63.5, CISPR 16-1-6: Reference Antenna Method, Horizontal/Vertical Polarization	3 Meter	(0 to 110) dB (20 to 72.5) MHz (72.5 to 115) MHz (115 to 157.5) MHz (157.5 to 200) MHz (200 to 300) MHz	0.95 dB 0.55 dB 0.41 dB 0.5 dB 0.6 dB
ANSI C63.5, CISPR 16-1-6: Identical Antenna Method, horizontal/vertical	3 Meter	(0 to 110) dB (20 to 72.5) MHz (72.5 to 115) MHz (115 to 157.5) MHz (157.5 to 200) MHz (200 to 300) MHz	0.96 dB 0.6 dB 0.39 dB 0.47 dB 0.52 dB
ANSI C63.5, CISPR 16-1-6: Standard Antenna Method, Horizontal/Vertical Polarization	3 Meter	(0 to 110) dB (20 to 300) MHz	0.5 dB
ANSI C63.5, CISPR 16-1-6: Three Antenna Method, Horizontal/Vertical Polarization	3 Meter	(0 to 110) dB (20 to 300) MHz	0.4 dB
ANSI C63.5, CISPR 16-1-6: Standard Site Method, Horizontal/Vertical Polarization	10 Meter	(0 to 110) dB (20 to 72.5) MHz (72.5 to 115) MHz (115 to 157.5) MHz (157.5 to 200) MHz (200 to 300) MHz	0.93 dB 0.52 dB 0.24 dB 0.2 dB 0.25 dB
ANSI C63.5, CISPR 16-1-6 Reference Antenna Method, Horizontal/Vertical Polarization	10 Meter	(0 to 110) dB (20 to 72.5) MHz (72.5 to 115) MHz (115 to 157.5) MHz (157.5 to 200) MHz (200 to 300) MHz	0.97 dB 0.62 dB 0.41 dB 0.3 dB 0.31 dB
ANSI C63.5, CISPR 16-1-6: Identical Antenna Method, Horizontal/Vertical Polarization	10 Meter	(0 to 110) dB (20 to 72.5) MHz (72.5 to 115) MHz (115 to 157.5) MHz (157.5 to 200) MHz (200 to 300) MHz	0.96 dB 0.6 dB 0.38 dB 0.46 dB 0.52 dB
ANSI C63.5, CISPR 16-1-6: Standard Antenna Method, Horizontal/Vertical Polarization	10 Meter	(0 to 110) dB (20 to 300) MHz	0.52 dB

**Electrical – RF/Microwave**

Kimballton, IA

<b>Parameter/Equipment</b>	Biconical Antennas		
<b>Reference Standard</b>	Calibration Test Site (CALTS) / Open Area Test Site (OATS), Keysight E5071C, N5225A, E8364B Network Analyzers		
<b>Method</b>	<b>Distance/ Domain</b>	<b>Frequency Range</b>	<b>Expanded Uncertainty of Measurement (+/-)</b>
ANSI C63.5, CISPR 16-1-6: Three Antenna Method, Horizontal/Vertical Polarization	10 Meter	(0 to 110) dB (20 to 300) MHz	0.43 dB

**Electrical – RF/Microwave**

Kimballton, IA

<b>Parameter/Equipment</b>	Log-Periodic Antennas - Horns		
<b>Reference Standard</b>	Calibration Test Site (CALTS) / Open Area Test Site (OATS), Fully Anechoic Room (FAR), Keysight E5071C, N5225A, E8364B Network Analyzers		
<b>Method</b>	<b>Distance/ Domain</b>	<b>Range</b>	<b>Expanded Uncertainty of Measurement (+/-)</b>
SAE ARP 958	1 Meter	(0 to 110) dB (140 to 400) MHz (400 to 1 000) MHz (1 000 to 5 000) MHz	0.32 dB 0.38 dB 0.52 dB
SAE ARP 958: Appendix C	3 Meter	(0 to 110) dB (140 to 400) MHz (400 to 1 000) MHz (1 000 to 5 000) MHz	0.38 dB 0.45 dB 0.58 dB
ANSI C63.5, CISPR 16-1-6: Standard Site Method, Horizontal/Vertical Polarization	3 Meter	(0 to 110) dB (140 to 300) MHz (300 to 400) MHz (400 to 500) MHz (500 to 600) MHz (600 to 700) MHz (700 to 800) MHz (800 to 900) MHz (900 to 1 000) MHz (1 000 to 5 000) MHz	0.3 dB 0.3 dB 0.4 dB 0.4 dB 0.4 dB 0.5 dB 0.5 dB 0.6 dB 0.7 dB

**Electrical – RF/Microwave**

Kimballton, IA

Parameter/Equipment	Log-Periodic Antennas - Horns		
Reference Standard	Calibration Test Site (CALTS) / Open Area Test Site (OATS), Fully Anechoic Room (FAR), Keysight E5071C, N5225A, E8364B Network Analyzers		
Method	Distance/ Domain	Range	Expanded Uncertainty of Measurement (+/-)
ANSI C63.5, CISPR 16-1-6: Identical Antenna Method, Horizontal/Vertical Polarization	3 Meter	(0 to 110) dB (140 to 300) MHz (300 to 400) MHz (400 to 500) MHz (500 to 600) MHz (600 to 700) MHz (700 to 800) MHz (800 to 900) MHz (900 to 1 000) MHz (1 000 to 5 000) MHz	0.2 dB 0.2 dB 0.2 dB 0.25 dB 0.35 dB 0.45 dB 0.45 dB 0.5 dB 0.6 dB
ANSI C63.5, CISPR 16-1-6: Standard Antenna Method, Horizontal/Vertical Polarization	3 Meter	(0 to 110) dB (140 to 5 000) MHz	0.65 dB
ANSI C63.5, CISPR 16-1-6: Three Antenna Method, Horizontal/Vertical Polarization	3 Meter	(0 to 110) dB (140 to 5 000) MHz	0.46 dB
ANSI C63.5, CISPR 16-1-6: Standard Site Method, Horizontal/Vertical Polarization	10 Meter	(0 to 110) dB (140 to 300) MHz (300 to 400) MHz (400 to 500) MHz (500 to 600) MHz (600 to 700) MHz (700 to 800) MHz (800 to 900) MHz (900 to 1 000) MHz (1 000 to 5 000) MHz	0.3 dB 0.3 dB 0.4 dB 0.4 dB 0.4 dB 0.5 dB 0.5 dB 0.5 dB 0.6 dB 0.7 dB
ANSI C63.5, CISPR 16-1-6: Identical Antenna Method	10 Meter	(0 to 110) dB (140 to 300) MHz (300 to 400) MHz (400 to 500) MHz (500 to 600) MHz (600 to 700) MHz (700 to 800) MHz (800 to 900) MHz (900 to 1 000) MHz	0.3 dB 0.3 dB 0.3 dB 0.3 dB 0.45 dB 0.45 dB 0.55 dB 0.6 dB



ANSI National Accreditation Board

Electrical – RF/Microwave

Kimballton, IA

Parameter/Equipment	Log-Periodic Antennas - Horns		
Reference Standard	Calibration Test Site (CALTS) / Open Area Test Site (OATS), Fully Anechoic Room (FAR), Keysight E5071C, N5225A, E8364B Network Analyzers		
Method	Distance/ Domain	Range	Expanded Uncertainty of Measurement (+/-)
		(1 000 to 5 000) MHz	0.7 dB
ANSI C63.5, CISPR 16-1-6: Standard Antenna Method, Horizontal/Vertical Polarization	10 Meter	(0 to 110) dB (140 to 5 000) MHz	0.69 dB
ANSI C63.5, CISPR 16-1-6: Three Antenna Method, Horizontal/Vertical Polarization	10 Meter	(0 to 110) dB (140 to 5 000) MHz	0.5 dB

Electrical – RF/Microwave

Kimballton, IA

Parameter/Equipment	Hybrid Antennas		
Reference Standard	Calibration Test Site (CALTS) / Open Area Test Site (OATS), Fully Anechoic Room (FAR), Keysight E5071C, N5225A, E8364B Network Analyzers		
Method	Distance/ Domain	Range	Expanded Uncertainty of Measurement (+/-)
SAE ARP 958	1 Meter	(0 to 110) dB (20 to 70) MHz (70 to 200) MHz (200 to 400) MHz (400 to 1 000) MHz (1 000 to 6 000) MHz	0.5 dB 0.76 dB 0.91 dB 0.74 dB 0.75 dB





ANSI National Accreditation Board

Electrical – RF/Microwave

Kimballton, IA

Parameter/Equipment	Hybrid Antennas		
Reference Standard	Calibration Test Site (CALTS) / Open Area Test Site (OATS), Fully Anechoic Room (FAR), Keysight E5071C, N5225A, E8364B Network Analyzers		
Method	Distance/ Domain	Range	Expanded Uncertainty of Measurement (+/-)
SAE ARP958: Appendix C	3 Meter	(0 to 110) dB (20 to 70) MHz (70 to 200) MHz (200 to 400) MHz (400 to 1 000) MHz (1 000 to 6 000) MHz	0.11 dB 0.11 dB 0.19 dB 0.26 dB 0.41 dB
ANSI C63.5, CISPR 16-1-6: Standard Site Method	3 Meter	(0 to 110) dB (20 to 1000) MHz (1 000 to 6 000) MHz	0.58 dB 0.75 dB
ANSI C63.5, CISPR 16-1-6: Standard Antenna Method	3 Meter	(0 to 110) dB (20 to 6 000) MHz	0.74 dB
ANSI C63.5, CISPR 16-1-6: Three Antenna Method	3 Meter	(0 to 110) dB (20 to 6 000) MHz	0.46 dB
ANSI C63.5, CISPR 16-1-6: Standard Site Method, Horizontal/Vertical Polarization	10 Meter	(0 to 110) dB (20 to 1 000) MHz (1 000 to 6 000) MHz	0.58 dB 0.75 dB
ANSI C63.5, CISPR 16-1-6: Identical Antenna Method, Horizontal/Vertical Polarization	10 Meter	(0 to 110) dB (20 to 1 000) MHz (1 000 to 6 000) MHz	0.68 dB 0.89 dB
ANSI C63.5, CISPR 16-1-6: Standard Antenna Method	10 Meter	(0 to 110) dB (20 to 6 000) MHz	0.77 dB
ANSI C63.5, CISPR 16-1-6: Three Antenna Method	10 Meter	(0 to 110) dB (20 to 6 000) MHz	0.5 dB



ANSI National Accreditation Board

**Electrical – RF/Microwave**

Kimballton, IA

Parameter/Equipment	Conical Log Spiral Antennas		
Reference Standard	Calibration Test Site (CALTS) / Open Area Test Site (OATS), Fully Anechoic Room (FAR), Keysight E5071C, N5225A, E8364B Network Analyzers		
Method	Distance/Domain	Frequency Range	Expanded Uncertainty of Measurement (+/-)
SAE ARP 958	1 Meter	(0 to 110) dB (200 to 400) MHz (400 to 1 000) MHz (1 000 to 10 000) MHz	2.2 dB 0.88 dB 1.7 dB

**Electrical – RF/Microwave**

Kimballton, IA

Parameter/Equipment	Loop Antennas	
Reference Standard	Electromagnetic Shielded Enclosure, Keysight E4445A Spectrum Analyzer	
Method	Range	Expanded Uncertainty of Measurement (+/-)
Standard field using Vacuo junction	(0 to 110) dB 5 Hz to 30 MHz	0.32 dB
ANSI C63.5, CISPR 16-1-6: Three Antenna Method	(0 to 110) dB 5 Hz to 30 MHz	0.5 dB
Standard field using loop current measurement	(0 to 110) dB 5 Hz to 30 MHz	0.34 dB
Substitution method using reference antenna	(0 to 110) dB 5 Hz to 30 MHz	0.44 dB

**Electrical – RF/Microwave**

Kimballton, IA

Parameter/Equipment	Rod Antennas	
Reference Standard	Keysight E5061B, E5071C Network Analyzers	
Method	Range	Expanded Uncertainty of Measurement (+/-)
CISPR 25, ANSI C63.5, SAE ARP 958, CISPR 16-1-4, CISPR 16-1-6: Equivalent Capacitance Substitution Method (ECSM)	(0 to 110) dB 10 Hz to 60 MHz	0.23 dB



ANSI National Accreditation Board

Electrical – RF/Microwave

Kimballton, IA

Parameter/Equipment	Additional Antenna Parameters	
Reference Standard	Calibration Test Site (CALTS) / Open Area Test Site (OATS), Fully Anechoic Room (FAR), Open Ended Anechoic Room, Keysight E5071C, N5225A, E8364B Network Analyzers	
Method	Range	Expanded Uncertainty of Measurement (+/-)
ANSI C63.5 4.4, CISPR 16-1-6: Symmetry	(0 to 110) dB 300 kHz to 1 GHz 10 MHz to 18 GHz (18 to 40) GHz	0.07 dB 0.05 dB 0.084 dB
CISPR 16-1-4, CISPR 16-1-6: Balance	(0 to 110) dB 20 MHz to 40 GHz	0.09 dB
CISPR 16-1-4, CISPR 16-1-6: Electric Field Discrimination	(0 to 110) dB 5 Hz to 30 MHz	0.13 dB
CISPR 16-1-4, CISPR 16-1-6: Cross-Polar Response	(0 to 110) dB 20 MHz to 40 GHz	0.5 dB
ANSI C63.4, CISPR 16-1-4, CISPR 16-1-6, IEEE 149-1979: VSWR	(0 to 110) dB (20 to 2000) MHz (1 to 40) GHz	0.6 dB 0.9 dB
CISPR 16-1-6: Pattern Measurements	(0 to 110) dB 1 MHz to 40 GHz	0.25 dB

Electrical – RF/Microwave

Kimballton, IA

Parameter/Equipment	Antenna Site Parameters <sup>1</sup>	
Reference Standard	Keysight E5071C, N5225A, E8364B Network Analyzers	
Method	Range	Expanded Uncertainty of Measurement (+/-)
ANSI C63.4, CISPR 16-1-4, CISPR 16-1-5, EN 50147-2: Normalized Site Attenuation (NSA)	(0 to 110) dB (30 to 1000) MHz	0.1 dB
ANSI C63.4, CISPR 16-1-4, CISPR 16-1-5: Site VSWR	(0 to 110) dB (1 to 6) GHz (6 to 18) GHz	0.66 dB 0.84 dB


**Length – Dimensional Metrology**

Kimballton, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Pin Depth	(0.18 to 0.23) in	34 $\mu$ in	Comparison to Maury Microwave A020D

[Return to Site listing \(top\)](#)

[Go to Notes \(bottom\)](#)

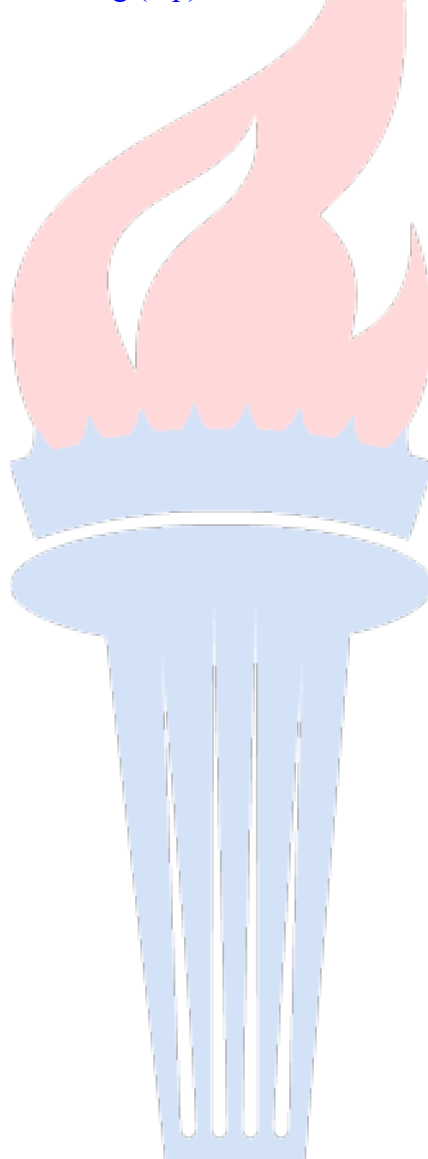



ANSI National Accreditation Board

### Services performed at satellite laboratory

2012 High Street  
Elk Horn, IA 51531

Nate Potts 712-248-6069  
[nate.potts@keysight.com](mailto:nate.potts@keysight.com) [www.keysight.com](http://www.keysight.com)

#### Electrical – DC/Low Frequency

Elk Horn, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
DC Voltage – Source	Up to 220 mV 220 mV to 2.2 V (2.2 to 11) V (11 to 22) V (22 to 220) V 220 V to 1.1 kV	7 $\mu$ V/V + 0.54 $\mu$ V 5 $\mu$ V/V + 0.8 $\mu$ V 3.5 $\mu$ V/V + 0.4 $\mu$ V 3.6 $\mu$ V/V + 4.5 $\mu$ V 5.3 $\mu$ V/V + 23 $\mu$ V 7.1 $\mu$ V/V + 0.3 mV	Comparison to Fluke 5720A or 5730A Multiproduct Calibrator with Fluke 5725A Amplifier
DC Voltage – Source Fixed Values	1 mV 10 mV	15 $\mu$ V 110 nV	Comparison to Fluke 57x0A Calibrator Fluke 742A Resistors
DC Voltage – Source Fixed Values	100 mV 1 V 10 V 100 V 1 000 V	270 nV 1.5 $\mu$ V 11 $\mu$ V 150 $\mu$ V 5.3 mV	Comparison to Fluke 57x0A Multiproduct Calibrator disciplined with HP Keysight 3458A multimeter/100 NPLC Option 002 Multimeter
DC Voltage – Measure	(0 to 0.1) V (0.1 to 1) V (1 to 10) V (10 to 100) V (100 to 1 000) V	4.1 $\mu$ V/V + 0.36 $\mu$ V 3.7 $\mu$ V/V + 0.35 $\mu$ V 3.1 $\mu$ V/V + 0.59 $\mu$ V 5.3 $\mu$ V + 36 $\mu$ V 5.3 $\mu$ V/V + 0.12 mV	Comparison to Keysight 3458A multimeter/100 NPLC Option 002 Multimeter
DC Voltage Transfer – Measure	(0 to 0.1) V (0.1 to 1) V (1 to 10) V (10 to 100) V (100 to 1 000) V	0.62 $\mu$ V/V + 62 nV 0.37 $\mu$ V/V + 124 nV 62 nV/V + 0.62 $\mu$ V 0.62 $\mu$ V/V + 12 $\mu$ V 1.9 $\mu$ V/V + 63 $\mu$ V	Comparison to Keysight 3458A multimeter
DC Current – Source	(>0 to 220) $\mu$ A 220 $\mu$ A to 22 mA (22 to 100) mA (100 to 220) mA 220 mA to 1 A (1 to 2.2) A	35 $\mu$ A/A 29 $\mu$ A/A 37 $\mu$ A/A 50 $\mu$ A/A - 1.2 $\mu$ A 59 $\mu$ A/A + 12 $\mu$ A 120 $\mu$ A/A - 42 $\mu$ A	Comparison to Fluke 5720A or 5730A Multiproduct Calibrator



ANSI National Accreditation Board

Electrical – DC/Low Frequency

Elk Horn, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
DC Current – Source	(2.2 to 11) A	0.28 mA/A + 41 $\mu$ A	Comparison to Fluke 5720A or 5730A Multiproduct Calibrator with Fluke 5725A Amplifier
DC Current – Source	100 $\mu$ A 1 mA 10 mA 100 mA 1 A	1.3 nA 9.5 nA 93 nA 2.2 $\mu$ A 36 $\mu$ A	Comparison to Fluke 57x0A Multiproduct Calibrator disciplined with HP Keysight 3458A multimeter/100 NPLC Option 002 Multimeter
DC Current – Source	(10 to 20) A (20 to 200) A (200 to 1 000) A	0.57 % of reading + 21 mA 0.57 % of reading + 145 mA 0.57 % of reading + 510 mA	Comparison to Fluke 5520A Multiproduct Calibrator, Fluke Current Coil
DC Current – Measure	(0 to 100) nA (0.1 to 1) $\mu$ A (1 to 10) $\mu$ A (10 to 100) $\mu$ A (0.1 to 1) mA (1 to 10) mA (10 to 100) mA (0.1 to 1) A	42 $\mu$ A/A + 50 pA 21 $\mu$ A/A + 50 pA 25 $\mu$ A/A + 0.11 nA 25 $\mu$ A/A + 0.85 nA 22 $\mu$ A/A + 6.4 nA 23 $\mu$ A/A + 59 nA 41 $\mu$ A/A + 0.6 $\mu$ A 125 $\mu$ A/A + 12 $\mu$ A	Comparison to Keysight 3458A multimeter
DC Current – Measure	(0.10 to 1.0) A (1.0 to 3.0) A (3.0 to 10) A	22 $\mu$ A/A + 61 $\mu$ A 38 $\mu$ A/A + 0.80 mA 0.02 % of reading + 1.9 mA	Comparison to Keysight 34470A Multimeter
DC Current – Measure	(1.0 to 2.0) A (2.0 to 10) A (10 to 20) A (20 to 50) A	0.016 % of reading - 0.032 mA 90 $\mu$ A/A + 1.0 mA 0.047 % of reading - 2.7 mA 0.048 % of reading - 2.7 mA	Comparison to PA2201A
DC Current – Measure	(20 to 500) A	0.09 % of reading	Comparison to 500 A shunts

**Electrical – DC/Low Frequency**

Elk Horn, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Resistance – Source Fixed Points	0 W	0.25 mΩ	Comparison to Fluke 5730A Multiproduct Calibrator
	1 W	0.27 mΩ	
	1.9 W	0.31 mΩ	
	10 W	0.34 mΩ	
	19 W	2.5 mΩ	
	100 W	2.7 mΩ	
	190 W	3.3 mΩ	
	1 kW	9.3 mΩ	
	1.9 kW	31 mΩ	
	10 kW	93 mΩ	
	19 kW	0.19 Ω	
	100 kW	1.2 Ω	
	190 kW	2.2 Ω	
	1 MW	20 Ω	
1.9 MW	42 Ω		
Resistance – Source Fixed Points	10 MΩ	0.4 kΩ	Comparison to Fluke 5730A Multiproduct Calibrator
	19 MΩ	1.5 kΩ	
	100 MΩ	12 kΩ	
Resistance - Source Fixed Points	0 Ω	21 μΩ	Comparison to Fluke 57x0A Multiproduct Calibrator disciplined with Keysight 3458A multimeter
	10 Ω	49 μΩ	
	100 Ω	420 μΩ	
	1 kΩ	1.8 mΩ	
	10 kΩ	17 mΩ	
	100 kΩ	190 mΩ	
	1 MΩ	4.6 Ω	
	10 MΩ	140 Ω	
	100 MΩ	18 kΩ	
Resistance – Source	(0 to 11) Ω	33 μΩ/Ω + 8.3 mΩ	Comparison to Fluke 5520A Multiproduct Calibrator
	(11 to 110) Ω	25 μΩ/Ω + 12.5 mΩ	
	110 Ω to 1.1 kΩ	23 μΩ/Ω + 17 mΩ	
	(1.1 to 3.3) kΩ	23 μΩ/Ω + 170 mΩ	
	(3.3 to 11) kΩ	23 μΩ/Ω + 84 mΩ	
	(11 to 110) kΩ	23 μΩ/Ω + 0.84 Ω	
	110 kΩ to 1.1 MΩ	27 μΩ/Ω + 8 Ω	
	(1.1 to 3.3) MΩ	50 μΩ/Ω + 125 Ω	
	(3.3 to 11) MΩ	0.11 mΩ/Ω + 0.2 kΩ	
	(11 to 33) MΩ	0.21 mΩ/Ω + 2 kΩ	
	(33 to 110) MΩ	0.41 mΩ/Ω + 2.8 kΩ	
(110 to 330) MΩ	2.5 mΩ/Ω + 83 kΩ		
(330 to 1 100) MΩ	13 mΩ/Ω + 0.4 MΩ		

**Electrical – DC/Low Frequency**

Elk Horn, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Resistance – Source	(1 to 10) GΩ (10 to 100) GΩ	1.2 % of reading + 56 kΩ 1.2 % of reading + 0.56 MΩ	Comparison to IET HRRS-F-6, 2177 Decade Resistor
Resistance – Measure	(0 to 12) Ω (10 to 120) Ω 100 Ω to 1.2 kΩ (1 to 12) kΩ (10 to 120) kΩ 100 kΩ to 1.2 MΩ (1 to 12) MΩ (10 to 120) MΩ 100 Ω to 1.2 GΩ	18 μΩ/Ω + 60 μΩ 12 μΩ/Ω + 0.6 mΩ 9.6 μΩ/Ω + 0.6 mΩ 9.6 μΩ/Ω + 6 mΩ 9.6 μΩ/Ω + 60 mΩ 14.5 μΩ/Ω + 2.4 Ω 60 μΩ/Ω + 120 Ω 0.6 mΩ/Ω + 1.2 kΩ 6 mΩ/Ω + 12 kΩ	Comparison to Keysight 3458A Multimeter
Resistance – Measure Fixed Points	1 Ω 1.9 Ω 10 Ω 19 Ω 100 Ω 190 Ω 1 kΩ 1.9 kΩ 10 kΩ 19 kΩ 100 kΩ 190 kΩ 1 MΩ 1.9 MΩ 10 MΩ 19 MΩ 100 MΩ	12 μΩ 13 μΩ 47 μΩ 0.098 mΩ 0.32 mΩ 0.55 mΩ 2.8 mΩ 3.9 mΩ 19 mΩ 57 mΩ 0.29 Ω 0.7 Ω 4.2 Ω 9.4 Ω 50 Ω 0.24 kΩ 2.3 kΩ	Comparison to Keysight 3458A Multimeter
AC Voltage – Source	Up to 2.2 mV (10 to 20) Hz (20 to 40) Hz 40 Hz to 20 kHz (20 to 50) kHz (50 to 100) kHz (100 to 300) kHz (300 to 500) kHz 500 kHz to 1 MHz	250 μV/V + 4.1 μV 94 μV/V + 4.1 μV 83 μV/V + 4.1 μV 210 μV/V + 4.1 μV 520 μV/V + 4.1 μV 1.1 mV/V + 4.1 μV 1.5 mV/V + 4.1 μV 2.8 mV/V + 4.1 μV	Comparison to Fluke 5730A Multiproduct Calibrator

**Electrical – DC/Low Frequency**

Elk Horn, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
AC Voltage – Source	Up to 22 mV		Comparison to Fluke 5730A Multiproduct Calibrator
	(10 to 20) Hz	250 $\mu\text{V}/\text{V}$ + 4.1 $\mu\text{V}$	
	(20 to 40) Hz	94 $\mu\text{V}/\text{V}$ + 4.1 $\mu\text{V}$	
	40 Hz to 20 kHz	83 $\mu\text{V}/\text{V}$ + 4.1 $\mu\text{V}$	
	(20 to 50) kHz	210 $\mu\text{V}/\text{V}$ + 4.1 $\mu\text{V}$	
	(50 to 100) kHz	520 $\mu\text{V}/\text{V}$ + 4.1 $\mu\text{V}$	
	(100 to 300) kHz	1.1 mV/V + 4.1 $\mu\text{V}$	
	(300 to 500) kHz	1.4 mV/V + 4.1 $\mu\text{V}$	
	500 kHz to 1 MHz	2.8 mV/V + 4.1 $\mu\text{V}$	
	(22 to 220) mV		
	(10 to 20) Hz	250 $\mu\text{V}/\text{V}$ + 39 $\mu\text{V}$	
	(20 to 40) Hz	94 $\mu\text{V}/\text{V}$ + 16 $\mu\text{V}$	
	40 Hz to 20 kHz	60 $\mu\text{V}/\text{V}$ + 7 $\mu\text{V}$	
	(20 to 50) kHz	120 $\mu\text{V}/\text{V}$ + 8 $\mu\text{V}$	
	(50 to 100) kHz	320 $\mu\text{V}/\text{V}$ + 18 $\mu\text{V}$	
	(100 to 300) kHz	680 $\mu\text{V}/\text{V}$ + 20 $\mu\text{V}$	
	(300 to 500) kHz	1.5 mV/V + 20 $\mu\text{V}$	
	500 kHz to 1 MHz	2.8 mV/V + 50 $\mu\text{V}$	
	220 mV to 2.2 V		
	(10 to 20) Hz	250 mV/V + 39 $\mu\text{V}$	
	(20 to 40) Hz	94 $\mu\text{V}/\text{V}$ + 16 $\mu\text{V}$	
	40 Hz to 20 kHz	43 $\mu\text{V}/\text{V}$ + 8.8 $\mu\text{V}$	
	(20 to 50) kHz	70 $\mu\text{V}/\text{V}$ + 10 $\mu\text{V}$	
	(50 to 100) kHz	89 $\mu\text{V}/\text{V}$ + 30 $\mu\text{V}$	
	(100 to 300) kHz	350 $\mu\text{V}/\text{V}$ + 83 $\mu\text{V}$	
	(300 to 500) kHz	1.1 mV/V + 190 $\mu\text{V}$	
	500 kHz to 1 MHz	1.8 mV/V + 300 $\mu\text{V}$	
	(2.2 to 22) V		
(10 to 20) Hz	251 $\mu\text{V}/\text{V}$ + 390 $\mu\text{V}$		
(20 to 40) Hz	93 $\mu\text{V}/\text{V}$ + 156 $\mu\text{V}$		
40 Hz to 20 kHz	47 $\mu\text{V}/\text{V}$ + 48 $\mu\text{V}$		
(20 to 50) kHz	78 $\mu\text{V}/\text{V}$ + 107 $\mu\text{V}$		
(50 to 100) kHz	113 $\mu\text{V}/\text{V}$ + 42 $\mu\text{V}$		
(100 to 300) kHz	432 $\mu\text{V}/\text{V}$ + 97 $\mu\text{V}$		
(300 to 500) kHz	1 mV/V + 2.1 mV		
500 kHz to 1 MHz	1.6 mV/V + 3.3 mV		

**Electrical – DC/Low Frequency**

Elk Horn, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
AC Voltage – Source	(22 to 220) V (10 to 20) Hz (20 to 40) Hz 40 Hz to 20 kHz (20 to 50) kHz (50 to 100) kHz (100 to 300) kHz (300 to 500) kHz 500 kHz to 1 MHz (220 to 1 100) V (15 to 50) Hz 50 Hz to 1 kHz	250 $\mu\text{V/V} + 4.2 \text{ mV}$ 94 $\mu\text{V/V} + 1.6 \text{ mV}$ 54 $\mu\text{V/V} + 0.68 \text{ mV}$ 83 $\mu\text{V/V} + 1.1 \text{ mV}$ 156 $\mu\text{V/V} + 2.6 \text{ mV}$ 941 $\mu\text{V/V} + 16 \text{ mV}$ 4.6 $\text{mV/V} + 42 \text{ mV}$ 8.3 $\text{mV/V} + 83 \text{ mV}$ 313 $\mu\text{V/V} + 17 \text{ mV}$ 73 $\mu\text{V/V} + 3.7 \text{ mV}$	Comparison to Fluke 5730A Multiproduct Calibrator
AC Voltage – Source	(220 to 1 100) V 40 Hz to 1 kHz (1 to 20) kHz (20 to 30) kHz (250 to 750) V (30 to 50) kHz (50 to 100) kHz	80 $\mu\text{V/V} + 18 \text{ mV}$ 173 $\mu\text{V/V} + 5.3 \text{ mV}$ 625 $\mu\text{V/V} + 12 \text{ mV}$ 634 $\mu\text{V/V} + 5.5 \text{ mV}$ 2.4 $\text{mV/V} + 28 \text{ mV}$	Comparison to Fluke 5730A Multiproduct Calibrator with Fluke 5725A Amplifier
AC Voltage – Source	0.01 V 1 kHz 20 kHz 100 kHz 300 kHz 1 MHz 4 MHz 0.1 V 1 kHz 20 kHz 100 kHz 300 kHz 1 MHz 4 MHz 8 MHz 10 MHz	870 nV 1.2 $\mu\text{V}$ 4.5 $\mu\text{V}$ 33 $\mu\text{V}$ 21 $\mu\text{V}$ 140 $\mu\text{V}$ 4.6 $\mu\text{V}$ 6.9 $\mu\text{V}$ 36 $\mu\text{V}$ 52 $\mu\text{V}$ 170 $\mu\text{V}$ 670 $\mu\text{V}$ 690 $\mu\text{V}$ 2.3 mV	Comparison to Fluke 5700A or Fluke 5720A Multiproduct Calibrator disciplined with Keysight 3458A Multimeter

Electrical – DC/Low Frequency

Elk Horn, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
AC Voltage – Source	1 V		Comparison to Fluke 5700A or Fluke 5720A Multiproduct Calibrator disciplined with Keysight 3458A Multimeter
	1 kHz	26 $\mu$ V	
	20 kHz	32 $\mu$ V	
	50 kHz	59 $\mu$ V	
	100 kHz	170 $\mu$ V	
	300 kHz	410 $\mu$ V	
	500 kHz	0.97 mV	
	1 MHz	1.7 mV	
	4 MHz	6.7 mV	
	8 MHz	6.9 mV	
	10 MHz	25 mV	
	3V		
	100 kHz	420 $\mu$ V	
	(2, 4, 8) MHz	21 mV	
	10 MHz	75 mV	
	10 V		
	10 Hz	480 $\mu$ V	
	20 Hz	270 $\mu$ V	
	40 Hz	230 $\mu$ V	
	200 Hz	460 $\mu$ V	
	500 Hz	495 $\mu$ V	
	1 kHz	260 $\mu$ V	
	10 kHz	270 $\mu$ V	
	20 kHz	320 $\mu$ V	
	50 kHz	0.53 mV	
	100 kHz	1.1 mV	
	300 kHz	2.6 mV	
	500 kHz	6.3 mV	
1 MHz	12 mV		
100 V			
1 kHz	4 mV		
20 kHz	7.9 mV		
50 kHz	7.5 mV		
100 kHz	16 mV		
700 V			
1 kHz	60 mV		



ANSI National Accreditation Board

Electrical – DC/Low Frequency

Elk Horn, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
AC Voltage Flatness – Source	300 $\mu$ V to 3.5 V (10 to 30) Hz	2.7 mV/V	Comparison to Fluke 5720A, Fluke 5700A, or Fluke 5700A-03 Multiproduct Calibrator (referenced to 1 kHz)
	30 Hz to 120 kHz	1.4 mV/V	
	300 $\mu$ V to 1.1 mV 120 kHz to 2 MHz	4.6 mV/V	
	(2 to 10) MHz	6.2 mV/V	
	(10 to 20) MHz	8 mV/V	
	(20 to 30) MHz	24 mV/V	
	1.1 $\mu$ V to 3 mV 120 kHz to 2 MHz	2.2 mV/V	
	(2 to 10) MHz	3.7 mV/V	
	(10 to 20) MHz	5.5 mV/V	
	(20 to 30) MHz	14 mV/V	
AC Voltage Flatness – Measure	3 mV to 3.5 V 120 kHz to 2 MHz	1.3 mV/V	Comparison to Agilent 11049A, Agilent 11050A, Agilent 11051A Thermal Voltage Converters
	(2 to 10) MHz	2.1 mV/V	
	(10 to 20) MHz	3.9 mV/V	
	(20 to 30) MHz	8.7 mV/V	
	Up to 3 V 10 Hz	0.2 mV/V + 6.9 $\mu$ V	
	100 Hz	80 $\mu$ V/V + 5.5 $\mu$ V	
	(10, 30) kHz	80 $\mu$ V/V + 3.2 $\mu$ V	
	100 kHz	0.1 mV/V + 8 $\mu$ V	
	300 kHz	0.1 mV/V + 5.2 $\mu$ V	
	1 MHz	0.1 mV/V + 6.5 $\mu$ V	
3 MHz	1.3 mV/V + 59 $\mu$ V		
8 MHz	1.3 mV/V + 0.11 mV		
10 MHz	1.3 mV/V + 91 $\mu$ V		
20 MHz	2.5 mV/V + 0.21 mV		
30 MHz	2.5 mV/V + 0.24 mV		
50 MHz	6.1 mV/V + 0.34 mV		
70 MHz	9 mV/V + 0.24 mV		
80 MHz	11 mV/V + 0.79 mV		
100 MHz	13 mV/V + 0.94 mV		
AC Voltage Flatness – Measure	9 kHz to 2 GHz (-60 to 25) dBm	0.026 dB	Comparison to Agilent N1914A Power Meter, Agilent E9304A, Agilent 8491B Power Sensors, Keysight 3458A Multimeter

**Electrical – DC/Low Frequency**

Elk Horn, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
AC Voltage – Measure	Up to 10 mV		Comparison to Keysight 3458A Multimeter
	(1 to 40) Hz	0.3 mV/V + 3.1 $\mu$ V	
	40 Hz to 1 kHz	0.2 mV/V + 1.2 $\mu$ V	
	(1 to 20) kHz	0.3 mV/V + 1.7 $\mu$ V	
	(20 to 50) kHz	1 mV/V + 1.6 $\mu$ V	
	(50 to 100) kHz	5 mV/V + 1.3 $\mu$ V	
	(100 to 300) kHz	40 mV/V + 2.1 $\mu$ V	
	300 kHz to 1 MHz	12 mV/V + 6.6 $\mu$ V	
	(1 to 4) MHz	70 mV/V + 7.5 $\mu$ V	
	(4 to 8) MHz	20 mV/V + 8.2 $\mu$ V	
	(10 to 100) mV		
	(1 to 40) Hz	70 $\mu$ V/V + 4.1 $\mu$ V	
	40 Hz to 1 kHz	70 $\mu$ V/V + 2.1 $\mu$ V	
	(1 to 20) kHz	0.14 mV/V + 2.3 $\mu$ V	
	(20 to 50) kHz	0.3 V/V + 2.6 $\mu$ V	
	(50 to 100) kHz	0.8 mV/V + 2.3 $\mu$ V	
	(100 to 300) kHz	3 mV/V + 15 $\mu$ V	
	300 kHz to 1 MHz	10 mV/V + 28 $\mu$ V	
	(1 to 2) MHz	15 mV/V + 20 $\mu$ V	
	(2 to 4) MHz	40 mV/V + 74 $\mu$ V	
	(4 to 8) MHz	40 mV/V + 83 $\mu$ V	
	(8 to 10) MHz	0.15 V/V + 0.11 mV	
	100 mV to 1 V		
	(1 to 40) Hz	70 $\mu$ V/V + 41 $\mu$ V	
	40 Hz to 1 kHz	70 $\mu$ V/V + 21 $\mu$ V	
	(1 to 20) kHz	0.14 mV/V + 22 $\mu$ V	
	(20 to 50) kHz	0.3 mV/V + 22 $\mu$ V	
	(50 to 100) kHz	0.8 mV/V + 22 $\mu$ V	
(100 to 300) kHz	3 mV/V + 0.12 mV		
300 kHz to 1 MHz	10 mV/V + 0.3 mV		
(1 to 2) MHz	15 mV/V + 0.21 mV		
(2 to 4) MHz	40 mV/V + 0.73 mV		
(4 to 8) MHz	40 mV/V + 0.83 mV		
(8 to 10) MHz	0.15 V/V + 1 mV		

**Electrical – DC/Low Frequency**

Elk Horn, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
AC Voltage – Measure	(1 to 10) V		Comparison to Keysight 3458A Multimeter
	(1 to 40) Hz	70 $\mu$ V/V + 0.42 mV	
	40 Hz to 1 kHz	70 $\mu$ V/V + 0.22 mV	
	(1 to 20) kHz	0.14 mV/V + 0.24 mV	
	(20 to 50) kHz	0.3 mV/V + 0.25 mV	
	(50 to 100) kHz	0.8 mV/V + 0.22 mV	
	(100 to 300) kHz	3 mV/V + 1.1 mV	
	300 kHz to 1 MHz	10 mV/V + 1.1 mV	
	(1 to 2) MHz	15 mV/V + 1.1 mV	
	(2 to 4) MHz	40 mV/V + 7.1 mV	
	(4 to 8) MHz	40 mV/V + 8.1 mV	
	(8 to 10) MHz	0.15 mV/V + 11 mV	
	(10 to 100) V		
	(1 to 40) Hz	0.2 mV/V + 4.1 mV	
	40 Hz to 20 kHz	0.2 mV/V + 2.6 mV	
(20 to 50) kHz	0.35 mV/V + 2.4 mV		
(50 to 100) kHz	1.2 mV/V + 2.1 mV		
(100 to 300) kHz	4 mV/V + 11 mV		
300 kHz to 1 MHz	15 mV/V + 50 mV		
(100 to 750) V			
(1 to 40) Hz	0.4 mV/V + 31 mV		
40 Hz to 1 kHz	0.4 mV/V + 16 mV		
(1 to 20) kHz	0.6 mV/V + 16 mV		
(20 to 50) kHz	1.2 mV/V + 16 mV		
(50 to 100) kHz	3 mV/V + 15 mV		
AC Voltage – Measure	(500 to 1 000) V		Comparison to Keysight PA2201A Power Analyzer
	(1.0 to 100) Hz	92 $\mu$ V/V + 2.6 mV	
	(0.10 to 1.0) kHz	56 $\mu$ V/V + 1 mV	
	(1.0 to 10) kHz	54 $\mu$ V/V + 3 mV	
	(10 to 100) kHz	0.89 mV/V + 20 mV	
	(0.10 to 1.0) MHz	0.88 mV/V + 86 mV	

**Electrical – DC/Low Frequency**

Elk Horn, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
AC Current Source	Up to 220 $\mu$ A		Comparison to Fluke 5720A or 5730A Multiproduct Calibrator
	(10 to 20) Hz	230 $\mu$ A/A + 17 nA	
	(20 to 40) Hz	150 $\mu$ A/A + 10 nA	
	40 Hz to 1 kHz	108 $\mu$ A/A + 8.4 nA	
	(1 to 5) kHz	266 $\mu$ A/A + 12.5 nA	
	(5 to 10) kHz	915 $\mu$ A/A + 66 nA	
	220 $\mu$ A to 2.2 mA		
	(10 to 20) Hz	233 $\mu$ A/A + 42 nA	
	(20 to 40) Hz	150 $\mu$ A/A + 34 nA	
	40 Hz to 1 kHz	108 $\mu$ A/A + 34 nA	
	(1 to 5) kHz	183 $\mu$ A/A + 109 nA	
	(5 to 10) kHz	915 $\mu$ A/A + 655 nA	
	(2.2 to 22) mA		
	(10 to 20) Hz	233 $\mu$ A/A + 422 nA	
	(20 to 40) Hz	149 $\mu$ A/A + 342 nA	
	40 Hz to 1 kHz	108 $\mu$ A/A + 343 nA	
	(1 to 5) kHz	183 $\mu$ A/A + 588 nA	
	(5 to 10) kHz	915 $\mu$ A/A + 5 $\mu$ A	
	(22 to 220) mA		
	(10 to 20) Hz	233 $\mu$ A/A + 4.2 $\mu$ A	
(20 to 40) Hz	149 $\mu$ A/A + 3.4 $\mu$ A		
40 Hz to 1 kHz	108 $\mu$ A/A + 2.6 $\mu$ A		
(1 to 5) kHz	183 $\mu$ A/A + 3.4 $\mu$ A		
(5 to 10) kHz	915 $\mu$ A/A + 10 $\mu$ A		
220 mA to 2.2 A			
20 Hz to 1 kHz	249 $\mu$ A/A + 34 $\mu$ A		
(1 to 5) kHz	383 $\mu$ A/A + 83 $\mu$ A		
(5 to 10) kHz	5.8 mA/A + 166 $\mu$ A		
(2.2 to 11) A			
40 Hz to 1 kHz	332 $\mu$ A/A + 149 $\mu$ A		
(1 to 5) kHz	707 $\mu$ A/A + 320 $\mu$ A		
(5 to 10) kHz	2.8 mA/A + 600 $\mu$ A		
AC Current Source	(0 to 0.33) mA		Comparison to Fluke 552xA Multiproduct Calibrator
	(10 to 30) kHz	10 mA/A + 330 nA	
	(0.33 to 3.3) mA		
	(10 to 30) kHz	6.6 mA/A + 550 nA	
	(3.3 to 33) mA		
(10 to 30) kHz	2.7 mA/A + 2.7 $\mu$ A		
(33 to 330) mA			
(10 to 30) kHz	2.7 mA/A + 160 $\mu$ A		

**Electrical – DC/Low Frequency**

Elk Horn, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
AC Current Source	(2.2 to 20.5) A (45 to 100) Hz 100 Hz to 1 kHz (1 to 5) kHz	830 $\mu$ A/A + 4.2 mA 1.1 mA/A + 3.9 mA 21 mA/A + 1 mA	Comparison to Fluke 552xA Multiproduct Calibrator
AC Current – Source	(10 to 20) A (45 to 65) Hz (65 to 440) Hz (20 to 100) A (45 to 65) Hz (65 to 100) Hz (100 to 440) Hz (100 to 1 000) A (45 to 65) Hz (65 to 100) Hz (100 to 440) Hz	0.3 % of reading + 27 mA 0.33 % of reading + 50 mA 0.85 % of reading + 3.6 mA 0.85 % of reading + 29 mA 0.85 % of reading + 100 mA 0.85 % of reading + 3.6 mA 0.85 % of reading + 28 mA 1 % of reading + 0.25 A	Comparison to Fluke 5520A Multiproduct Calibrator, Fluke Current Coil
AC Current – Source	1 kHz 10 $\mu$ A 100 $\mu$ A 1 mA 10 mA 100 mA 1 A	7.3 nA 14 nA 85 nA 0.87 $\mu$ A 8.7 $\mu$ A 200 $\mu$ A	Comparison to Fluke 5720A or 5730A Multiproduct Calibrator disciplined with Keysight 3458A Multimeter
AC Current – Measure	Up to 100 $\mu$ A (10 to 20) Hz (20 to 45) Hz 45 Hz to 1 kHz 100 $\mu$ A to 1 mA (10 to 20) Hz (20 to 45) Hz 45 Hz to 1 kHz (1 to 10) mA (10 to 20) Hz (20 to 45) Hz 45 Hz to 1 kHz (10 to 100) mA (10 to 20) Hz (20 to 45) Hz 45 Hz to 1 kHz	4 mA/A + 31 nA 1.5 mA/A + 31 nA 0.6 mA/A + 31 nA 4 mA/A + 0.31 $\mu$ A 0.15 mA/A + 0.21 $\mu$ A 0.6 mA/A + 0.21 $\mu$ A 4 mA/A + 3.1 $\mu$ A 1.5 mA/A + 2.1 $\mu$ A 0.6 mA/A + 2.1 $\mu$ A 4 mA/A + 31 $\mu$ A 1.5 mA/A + 21 $\mu$ A 0.6 mA/A + 21 $\mu$ A	Comparison to Keysight 3458A Multimeter

**Electrical – DC/Low Frequency**

Elk Horn, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
AC Current – Measure	100 mA to 1.05 A (10 to 20) Hz (20 to 45) Hz (45 to 100) Hz 100 Hz to 5 kHz	4 mA/A + 0.22 mA 1.6 mA/A + 0.22 mA 0.8 mA/A + 0.22 mA 1 mA/A + 0.22 mA	Comparison to Keysight 3458A Multimeter
AC Current – Measure	(1 to 3) A 3.0 Hz to 5.0 kHz (5.0 to 10) kHz (3 to 10) A 3.0 Hz to 5.0 kHz (5.0 to 10) kHz	0.028 % of reading + 0.19 mA 0.044 % of reading + 0.37 mA 0.035 % of reading + 0.58 mA 0.076 % of reading + 0.63 mA	Comparison to Keysight 34470A Multimeter
AC Current – Measure	(1 to 2) A (1.0 to 100) Hz (0.10 to 1) kHz (1 to 10) kHz (10 to 100) kHz (2 to 50) A (1 to 100) Hz (0.1 to 1) kHz (1 to 10) kHz (10 to 100) kHz	0.01 % of reading + 73 $\mu$ A 0.021 % of reading + 8.0 $\mu$ A 0.11 % of reading + 19 $\mu$ A 0.11 % of reading + 20 $\mu$ A 0.044 % of reading + 1.9 mA 0.045 % of reading + 1.6 mA 0.046 % of reading + 2.3 mA 0.043 % of reading + 3.7 mA	Comparison to Keysight PA2201A Power Analyzer
Oscilloscope Calibration – Generate Voltage – DC to 1 MW DC to 50 W  Square Wave – 50 W  Rise Time  Timing	1 mV to 200 V 1 mV to 5 V  (0.04 to 1) mV 1 mV to 5 V  150 ps @ 5 mV to 3 V 70 ps @ 25 mV to 2 V 25 ps @ (425 to 575) mV  Narrow Triangle 900.91 ns to 55 s	0.03 % of reading + 25 $\mu$ V 0.03 % of reading + 25 $\mu$ V  1.5 % of reading + 10 $\mu$ V 0.12 % of reading + 10 $\mu$ V  27 ps 20 ps 8.1 ps  3.4 $\mu$ s/s	Comparison to Fluke 9500 oscilloscope calibration system, Fluke 9500B with 9530, 9550 and 9560 heads

**Electrical – DC/Low Frequency**

Elk Horn, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Oscilloscope Calibration – Leveled Sine Wave – Amplitude	4.44 mV to 5.56 V	1.5 % of reading	Comparison to Fluke 9500 oscilloscope calibration system, Fluke 9500B with 9530, 9550 and 9560 heads
Single	Flatness 0.1 Hz to 300 MHz (300 to 550) MHz 550 MHz to 3 GHz (3 to 6) GHz	2 % of reading 2.5 % of reading 3.5 % of reading 5 % of reading	
Dual	Flatness wrt Reference Frequency: 0.1 Hz to 1 GHz (1 to 3.2) GHz	10 % of reading 25 % of reading	
Pulse Width	(1 to 100) ns	5 % of reading + 200 ps	
Time Marker Output – Measuring Equipment	50 kHz to 2.5 GHz	0.004 % of reading	
Bandwidth Measurement	1 MHz to 2.5 GHz	2.3 % of reading	
Inductance – Measure	10 μH to 100 H (100, 120) Hz	0.1 % of reading + 1 μH	Comparison to GenRad 165 Digibridge Impedance Bridge
	1 μH to 10 H 1 kHz	0.1 % of reading + 0.1 μH	
	0.1 μH to 1 H 10 kHz	0.1 % of reading + 0.02 μH	
Capacitance – Source	(0.19 to 3.29) nF	3.1 mF/F + 7.7 pF	Comparison to Fluke 5520A or 5522A Multiproduct Calibrator
	(3.3 to 10.99) nF	1.4 mF/F + 8.2 pF	
	(11 to 109.99) nF	1.4 mF/F + 80 pF	
	(110 to 329.99) nF	1.5 mF/F + 0.24 nF	
	(0.33 to 1.099) μF	1.4 mF/F + 0.82 nF	

**Electrical – DC/Low Frequency**

Elk Horn, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Capacitance – Source	(1.1 to 3.299) $\mu$ F (3.3 to 10.99) $\mu$ F (11 to 32.99) $\mu$ F (33 to 109.99) $\mu$ F (110 to 329.99) $\mu$ F (0.33 to 1.099) mF (1.1 to 3.299) mF (3.3 to 10.00) mF (11 to 32.99) mF (33 to 110) mF	1.5 mF/F + 2.4 nF 1.4 mF/F + 8.1 nF 2.4 mF/F + 24 nF 2.6 mF/F + 83 nF 2.7 mF/F + 0.24 $\mu$ F 2.6 mF/F + 0.82 $\mu$ F 2.7 mF/F + 2.4 $\mu$ F 3.3 mF/F + 5.2 $\mu$ F 5.5 mF/F + 24 $\mu$ F 7.9 mF/F + 79 $\mu$ F	Comparison to Fluke 5520A or 5522A Multiproduct Calibrator
Capacitance – Measure	(10 to 100) pF (0.10 to 1) nF (1 to 100) nF (0.1 to 1.0) $\mu$ F (1 to 100) $\mu$ F (100 to 1 000) $\mu$ F (1 to 10) mF (10 to 100) mF	0.029 % of reading + 0.000 11 pF 0.026 % of reading + 0.029 pF 0.029 % of reading + 0.006 1 pF 0.015 % of reading + 0.000 31 nF 0.022 % of reading + 0.008 9 nF 0.029 % of reading + 0.000 55 $\mu$ F 0.029 % of reading + 0.005 4 $\mu$ F 0.029 % of reading + 0.054 $\mu$ F	Comparison to Keysight Technologies E4980A
Electrical Simulation of Thermocouple Indicating Devices	Type B (600 to 800) $^{\circ}$ C (800 to 1 000) $^{\circ}$ C (1 000 to 1 550) $^{\circ}$ C (1 550 to 1 820) $^{\circ}$ C Type C (0 to 150) $^{\circ}$ C (150 to 650) $^{\circ}$ C (650 to 1 000) $^{\circ}$ C (1 000 to 1 800) $^{\circ}$ C (1 800 to 2 316) $^{\circ}$ C Type E (-250 to -100) $^{\circ}$ C (-100 to -25) $^{\circ}$ C (-25 to 350) $^{\circ}$ C (350 to 650) $^{\circ}$ C 650 $^{\circ}$ C	0.47 $^{\circ}$ C 0.36 $^{\circ}$ C 0.32 $^{\circ}$ C 0.35 $^{\circ}$ C 0.32 $^{\circ}$ C 0.28 $^{\circ}$ C 0.33 $^{\circ}$ C 0.53 $^{\circ}$ C 0.88 $^{\circ}$ C 0.53 $^{\circ}$ C 0.18 $^{\circ}$ C 0.16 $^{\circ}$ C 0.18 $^{\circ}$ C 0.23 $^{\circ}$ C	Comparison to Fluke 5520A Fluke 5522A Multiproduct Calibrator

Electrical – DC/Low Frequency

Elk Horn, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Electrical Simulation of Thermocouple Indicating Devices	Type J		Comparison to Fluke 5520A Fluke 5522A Multiproduct Calibrator
	(-210 to -100) °C	0.29 °C	
	(-100 to -30) °C	0.18 °C	
	(-30 to 150) °C	0.16 °C	
	(150 to 760) °C	0.19 °C	
	(760 to 1 200) °C	0.25 °C	
	Type K		
	(-200 to -100) °C	0.35 °C	
	(-100 to -25) °C	0.2 °C	
	(-25 to 120) °C	0.18 °C	
	(120 to 1 000) °C	0.28 °C	
	(1 000 to 1 372) °C	0.42 °C	
	Type L		
	(-200 to -100) °C	0.39 °C	
	(-100 to 800) °C	0.28 °C	
	(800 to 900) °C	0.19 °C	
	Type N		
	(-200 to -100) °C	0.42 °C	
	(-100 to -25) °C	0.24 °C	
	(-25 to 120) °C	0.21 °C	
	(120 to 410) °C	0.2 °C	
	(410 to 1 300) °C	0.29 °C	
	Type R		
	(0 to 250) °C	0.6 °C	
	(250 to 400) °C	0.37 °C	
	(400 to 1 000) °C	0.35 °C	
	(0 000 to 1 767) °C	0.42 °C	
	Type S		
(0 to 250) °C	0.5 °C		
(250 to 1 000) °C	0.38 °C		
(1 000 to 1 400) °C	0.39 °C		
(1 400 to 1 767) °C	0.49 °C		
Type T			
(-250 to -150) °C	0.66 °C		
(-150 to 0) °C	0.26 °C		
(0 to 120) °C	0.18 °C		
(120 to 400) °C	0.16 °C		
Type U			
(-200 to 0) °C	0.59 °C		
(0 to 600) °C	0.29 °C		

**Electrical – DC/Low Frequency**

Elk Horn, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
DC High Voltage – Measure and Source	(1 to 10) kV	44 $\mu$ V/V + 0.42 V	Comparison to Vitrek 4700 Precision High Voltage Meter
DC High Voltage – Measure and Source	(10 to 35) kV (35 to 50) kV (50 to 70) kV	20 $\mu$ V/V + 5.5 V 34 $\mu$ V/V + 11 V 47 $\mu$ V/V + 30 V	Comparison to Vitrek 4700 Precision High Voltage Meter and Probe Vitrek 4700 & HVP-35 Vitrek 4700 & HVL-70 Vitrek 4700 & HVL-70
AC High Voltage – Measure and Source	(DC to 1 kHz) (1.0 to 10) kV	0.013 % of reading + 2.6 V	Comparison to Vitrek 4700 Precision High Voltage Meter
AC High Voltage – Measure and Source	(DC to 1 kHz) (10 to 30) kV (30 to 50) kV	0.016 % of reading + 1.6 V 66 $\mu$ V/V + 13 V	Comparison to Vitrek 4700 Precision High Voltage Meter and Probe Vitrek 4700 & HVP-35 Vitrek 4700 & HVL-70

**Electrical – RF/Microwave**

Elk Horn, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Amplitude Modulation – Measure Rate: (0.05 to 10) kHz Rate: (0.05 to 50) kHz Rate: (0.05 to 10) kHz	Up to 99% Depth (0.15 to 10) MHz (0.01 to 1.3) GHz (1.3 to 26.5) GHz	2.1 % Depth 1.1 % Depth 1.6 % Depth	Comparison to Agilent 8902A Measuring Receiver
Frequency Modulation – Measure Rate: (0.02 to 10) kHz Rate: (0.05 to 100) kHz	$\leq$ 40 kHz <sub>peak</sub> (0.25 to 10) MHz $\leq$ 400 kHz <sub>peak</sub> (0.01 to 26.5) GHz	2.2 % Deviation 1.2 % Deviation	Comparison to HP 8902A Measuring Receiver
Digital Modulation RF Quality Error Vector Magnitude (EVM)	Mod Frequency Span: $f \leq$ 100 kHz $100 \text{ kHz} \leq f \leq 1 \text{ MHz}$ $f > 1 \text{ MHz}$	0.43 % of reading 0.48 % of reading 0.82 % of reading	Comparison to HP 89441A Vector Signal Analyzer

**Electrical – RF/Microwave**

Elk Horn, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Digital Modulation RF Quality Phase Error	Up to 180 ° Mod Frequency Span: f ≤ 100 kHz 100kHz ≤ f ≤ 1MHz f > 1 MHz	0.17 ° rms 0.34 ° rms 0.57 ° rms	Comparison to HP 89441A Vector Signal Analyzer
Digital Modulation RF Quality Frequency Error	(0 to 5) % error Mod Frequency 1 GHz 2 GHz 3 GHz 4 GHz 5 GHz 6 GHz	0.063 % error 0.068 % error 0.079 % error 0.099 % error 0.33 % error 0.39 % error	Comparison to HP 89441A Vector Signal Analyzer
Digital Modulation RF Quality Modulation Accuracy (Rho)	Mod Frequency Span: f ≤ 100 kHz 0.999 9 ≤ r ≤ 1 0.997 5 ≤ r < 0.999 9 0.993 6 ≤ r < 0.997 5 0.99 ≤ r < 0.993 6 0.978 ≤ r < 0.99 0.96 ≤ r < 0.978 100 kHz ≤ f ≤ 1 MHz 0.999 9 ≤ r ≤ 1 0.997 5 ≤ r < 0.999 9 0.993 6 ≤ r < 0.997 5 0.99 ≤ r < 0.993 6 0.978 ≤ r < 0.99 0.96 ≤ r < 0.978	8.6E <sup>-5</sup> r 0.000 43 r 0.000 68 r 0.000 84 r 0.001 2 r 0.001 6 r 9.6 E <sup>-5</sup> r 0.000 48 r 0.000 76 r 0.000 94 r 0.001 4 r 0.001 8 r	Comparison to HP 89441A Vector Signal Analyzer
Digital Modulation RF Quality Modulation Accuracy (Rho)	Mod Frequency Span: f > 1 MHz 0.999 9 ≤ r ≤ 1 0.997 5 ≤ r < 0.999 9 0.993 6 ≤ r < 0.997 5 0.99 ≤ r < 0.993 6 0.978 ≤ r < 0.99 0.96 ≤ r < 0.978	1.6 E <sup>-4</sup> r 0.000 82 r 0.001 3 r 0.001 6 r 0.002 4 r 0.003 r	Comparison to HP 89441A Vector Signal Analyzer



ANSI National Accreditation Board

Electrical – RF/Microwave

Elk Horn, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Phase Modulation – Measure	(0.15 to 10) MHz Rate: (0.02 to 10) kHz <40 Radians Deviation	4.1 % Deviation	Comparison to HP 8902A Measuring Receiver
	(0.01 to 26.5) GHz Rate: (0.2 to 20) kHz <400 Radians Deviation	3.1 % Deviation	
Phase Modulation – Measure	100 kHz to 6.6 GHz Deviations: (0.3 to 7) rad Deviations: > 7 rad	3.1 % Deviation 1 % Deviation	Comparison to Keysight E444xA with Opt. 233 Spectrum Analyzer
	(6.6 to 13.2) GHz Deviations: (0.6 to 2) rad	3.1 % Deviation	
	(13.2 to 26.5) GHz Deviations: > 2 rad	1 % Deviation	
	Deviations: (1.2 to 4) rad	3.1 % Deviation	
Distortion Measure	(-99.99 to 0) dB	1.2 dB	Comparison to HP 8903A/B Audio Analyzer
	20 Hz to 20 kHz (20 to 100) kHz	2.4 dB	
RF Power - Power Meter Reference	1 mW 50 MHz	0.23 % of reading	Comparison to Keysight N1914A or E4419A/B Power Meter and N8482A or 8482A Power Sensor
Tuned RF Power - Absolute – Measure 2.5 MHz to 26.5 GHz	(-22 to +10) dBm (-42 to -22) dBm (-50 to -42) dBm (-60 to -50) dBm (-72 to -60) dBm (-80 to -72) dBm (-92 to -80) dBm (-102 to -92) dBm (-110 to -102) dBm (-120 to -110) dBm (-127 to -120) dBm	0.17 dB 0.18 dB 0.2 dB 0.21 dB 0.22 dB 0.23 dB 0.24 dB 0.27 dB 0.28 dB 0.31 dB 0.34 dB	Comparison to HP 8902A Measuring Receiver with HP 11722A or with HP 11792A and HP 11793A Power Sensor

**Electrical – RF/Microwave**

Elk Horn, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Tuned RF Power - Relative – Measure  2.5 MHz to 26.5 GHz	(+2 to +10) dBm	0.08 dB	Comparison to HP 8902A Measuring Receiver with HP 11722A or with HP 11792A and HP 11793A Power Sensor
	(-12 to +2) dBm	0.07 dB	
	(-22 to -12) dBm	0.08 dB	
	(-31 to -22) dBm	0.09 dB	
	(-40 to -31) dBm	0.1 dB	
	(-50 to -40) dBm	0.12 dB	
	(-61 to -50) dBm	0.15 dB	
	(-71 to -61) dBm	0.16 dB	
	(-80 to -71) dBm	0.17 dB	
	(-90 to -80) dBm	0.19 dB	
	(-100 to -90) dBm	0.22 dB	
	(-110 to -100) dBm	0.23 dB	
(-120 to -110) dBm	0.27 dB		
(-127 to -120) dBm	0.3 dB		
RF Absolute Power - Source  50 MHz	(-11 to -1) dB	0.025 dB	Comparison to Signal Source and Step Attenuators PSG, ESG, 8496G/H and 8494G/H
	(-30 to -10) dB	0.025 dB	
	(-50 to -40) dB	0.027 dB	
	-60 dB	0.028 dB	
	(-90 to -70) dB	0.033 dB	
	-100 dB	0.04 dB	
-110 dB	0.048 dB		
RF Absolute Power – Source	0.02 V ≤ V < 7 V f < 10 MHz	0.082 dB	Comparison to Function Generator and DVM Agilent 33250A, Agilent 33120A, Agilent Keysight 3458A Multimeter
	10 MHz ≤ f ≤ 50 MHz	0.16 dB	
	50 MHz ≤ f ≤ 80 MHz	0.4 dB	
	V ≤ 10mV 20 Hz ≤ f ≤ 20 kHz	0.017 mV	
	20 kHz < f ≤ 50 kHz	0.021 mV	
	50 kHz < f ≤ 100 kHz	0.05 mV	
	100 kHz < f ≤ 300 kHz	0.38 mV	
RF Absolute Power – Source	10 mV < V ≤ 100 mV 20 Hz ≤ f ≤ 40 Hz	0.029 mV	Comparison to Function Generator and DVM, Agilent 33250A, Agilent 33120A, Agilent Keysight 3458A Multimeter
	40 Hz ≤ f ≤ 1 kHz	0.028 mV	
	1 kHz < f ≤ 20 kHz	0.032 mV	
	20 kHz < f ≤ 50 kHz	0.045 mV	
	50 kHz < f ≤ 100 kHz	0.08 mV	
	100 kHz < f ≤ 300 kHz	0.3 mV	

**Electrical – RF/Microwave**

Elk Horn, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
RF Absolute Power – Source	100 mV < V ≤ 1 V 20 Hz ≤ f ≤ 1 kHz 1 kHz < f ≤ 20 kHz 20 kHz < f ≤ 50 kHz 50 kHz < f ≤ 100 kHz 100 kHz < f ≤ 300 kHz 1 V < V ≤ 3.5 V 20 Hz ≤ f ≤ 40 Hz 40 Hz ≤ f ≤ 1 kHz 1 kHz < f ≤ 20 kHz 20 kHz < f ≤ 50 kHz 50 kHz < f ≤ 100 kHz 100 kHz < f ≤ 300 kHz	0.7 mV 0.72 mV 0.79 mV 1.3 mV 3.7 mV 2.2 mV 2.1 mV 2.2 mV 2.5 mV 4 mV 13 mV	Comparison to Function Generator and DVM, Agilent 33250A, Agilent 33120A, Agilent Keysight 3458A Multimeter
RF Absolute Power – Source	7 dBm ≥ P ≥ 0 dBm 0.3 MHz ≤ f ≤ 1.1 GHz 1.1 GHz ≤ f ≤ 2.985 GHz 2.985 GHz < f ≤ 4 GHz 4 GHz < f ≤ 6 GHz 0 dBm > P ≥ -25 dBm 0.3 MHz ≤ f ≤ 1.1 GHz 1.1 GHz ≤ f ≤ 2.985 GHz 2.985 GHz < f ≤ 4 GHz 4 GHz < f ≤ 6 GHz -25 dBm > P ≥ -70 dBm 0.3 MHz ≤ f ≤ 1.1 GHz 1.1 GHz ≤ f ≤ 2.985 GHz 2.985 GHz < f ≤ 4 GHz 4 GHz < f ≤ 6 GHz -70 dBm > P ≥ -95 dBm 0.3 MHz ≤ f ≤ 1.1 GHz 1.1 GHz ≤ f ≤ 2.985 GHz 2.985 GHz < f ≤ 4 GHz 4 GHz < f ≤ 6 GHz -95 dBm > P ≥ -125 dBm 0.3 MHz ≤ f ≤ 1.1 GHz 1.1 GHz ≤ f ≤ 2.985 GHz 2.985 GHz < f ≤ 4 GHz 4 GHz < f ≤ 6 GHz	0.49 dB 0.58 dB 0.69 dB 0.79 dB 0.49 dB 0.59 dB 0.69 dB 0.8 dB 0.5 dB 0.59 dB 0.69 dB 0.8 dB 0.5 dB 0.6 dB 0.7 dB 0.8 dB 0.51 dB 0.6 dB 0.7 dB 1.5 dB	Comparison to Signal Source PSG, ESG



ANSI National Accreditation Board

Electrical – RF/Microwave

Elk Horn, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Harmonic Measurements	(0 to 90) dB 30 Hz to 25 GHz 200 Hz to 80 MHz (10 to 25) GHz	0.5 dB 1.2 dB 0.8 dB	Comparison to Agilent 8565E Spectrum Analyzer Agilent 3335A Agilent 83650B (based on Agilent 8565E) Signal Generators
Source Errors for CISPR Impulse Spectral Amplitude	(-20 to 45) dB Band A (9 to 150) kHz Band B (0.15 to 30) MHz Band C and D (30 to 1 000) MHz	0.17 dB 0.22 dB 0.22 dB	CISPR 16-1-1 IGUU 2916 IGUU 2918 Pulse Generators
Source Errors for CISPR Impulse Spectral Amplitude	(-30 to 20) dB Band E (1 to 18) GHz	0.27 dB	Comparison to Agilent 83650B, Agilent 33250A Signal Generators
Source Errors for Sinewave Output	(40 to 80) dB Band A Band B Band C/D	0.17 dB 0.22 dB 0.22 dB	CISPR 16-1-1 IGUU 2916 IGUU 2918 Pulse Generators
Source Errors for Sinewave Output	(40 to 80) dB Band E	0.27 dB	Comparison to Agilent 83650B, Agilent 33250A Signal Generators
Relative Pulse Response	(0 to 40) dB Band A Band B Band C/D	0.17 dB 0.22 dB 0.22 dB	CISPR 16-1-1 IGUU 2916 IGUU 2918 Pulse Generators
Relative Pulse Response	(0 to 40) dB Band E	0.27 dB	Comparison to Agilent 83650B, Agilent 33250A Signal Generators
Impulse Flatness of Spectral Amplitude	(0 to 5) dB Band A Band B Band C/D	0.14 dB 0.13 dB 0.13 dB	CISPR 16-1-1 Agilent E4440 Spectrum Analyzer

**Electrical – RF/Microwave**

Elk Horn, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
EFT/Burst Generator – Voltage	10 V to 6 kV	0.7 % of reading	EN 61000-4-4; IEC 61000-4-4, IEC 61000-4-4(2004, 2011); GR 1089 CORE ISO 7637-2 Tektronix TDS 5104B Oscilloscope
Rise Time	5 ns	0.067 ns	
Impulse Duration	150 ns	0.095 ns	
Burst Duration	15 ms 0.75 ms	1.4 $\mu$ s 0.033 $\mu$ s	
Burst Period	300 ms	0.016 ms	
Repetition Rate	5.0 kHz 100 kHz	0.23 Hz 5 Hz	
Surge Generator – Ring/ Impulse/ PQF Front Time Open Short	(0.1 to 50) $\mu$ s	0.004 % of reading + 0.2 ns	IEC/EN61000-4-5; IEC/EN 61000-4-8; IEC/EN 61000-4-9; IEC/EN 61000-4-10; IEC/EN 61000-4-11; IEC/EN 61000-4-12 UL 864; UL 1449; ISO 7637-2
Rise Time Open Circuit Short Circuit	(0.1 to 50) $\mu$ s	0.004 % of reading + 0.2 ns	
Time to Half-Value Impulse Duration	(20 to 1 500) $\mu$ s	0.004 % of reading + 0.2 ns	
Surge Generator – Ring/ Impulse/ PQF Voltage	10 V to 6.0 kV (6.0 to 18) kV	0.7 % of reading 1.1 % of reading	ITU Rec K.17, K.20, ITU Rec K.21; SBC-TP-76200; GR1089CORE
Current	(0.001 to 5) kA	1.1 % of reading	
Surge Generator – Ring/ Impulse/ PQF Phase Synchronization	50 Hz 60 Hz 400 Hz	0.11 ° 0.095 ° 0.21 °	IEC/EN 61000-4-18 Tektronix TDS 5104B Oscilloscope PDP8000, P6015A,110 Voltage Probes ANSI C62.41
Mains Harmonic Emissions	(100 to 280) V (0.1 to 20) A (20 to 60) A (0.5 to 179.5)°	0.07 % of reading + 270 mV 0.2 % of reading 0.1 A 0.1°	IEC/EN 61000-3-2; IEC/EN 61000-4-7; IEC/EN 61000-4-13; IEC/EN 61000-4-14

**Electrical – RF/Microwave**

Elk Horn, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Voltage Fluctuations (Flicker)	(100 to 280) V (0.1 to 20) A (20 to 60) A	0.1 % of reading + 370 mV 0.2 % of reading 0.1 A	IEC/EN 61000-3-3 IEC/EN 61000-3-12 IEC/EN 61000-4-15

**Electrical – RF/Microwave**

Elk Horn, IA

Parameter/Equipment	Attenuation – Source <sup>1</sup>											
Reference Standard, Method, and/or Equipment	Comparison to 8494H Attenuator											
Range	Expanded Uncertainty of Measurement (+/-)											
Frequency Ranges	Step Attenuation Level in dB											
	1	2	3	4	5	6	7	8	9	10	11	
20 Hz ≤ f < 300 kHz	0.002 8	0.002 7	0.002 7	0.002 8	0.002 9	0.002 8	0.002 9	0.002 8	0.002 8	0.002 8	0.002 8	0.003 3
300 kHz ≤ f < 80 MHz	0.002 9	0.002 8	0.002 8	0.003	0.003	0.003	0.003	0.003 4	0.003 7	0.003 7	0.003 7	0.003 8
80 MHz ≤ f < 1 GHz	0.005 4	0.005 4	0.005 4	0.005 3	0.005 4	0.005 4	0.005 1	0.005 4	0.005 4	0.005 4	0.005 9	0.005 3
1 GHz ≤ f < 4 GHz	0.066	0.068	0.068	0.069	0.071	0.071	0.072	0.073	0.073	0.073	0.074	0.074
4 GHz ≤ f < 10 GHz	0.1	0.1	0.1	0.1	0.1	0.1	0.1	0.11	0.11	0.11	0.11	0.11
10 GHz ≤ f < 14 GHz	0.14	0.14	0.14	0.14	0.15	0.14	0.14	0.15	0.15	0.14	0.14	0.14
14 GHz ≤ f ≤ 18 GHz	0.19	0.18	0.19	0.17	0.2	0.19	0.19	0.19	0.18	0.19	0.19	0.2

**Electrical – RF/Microwave**

Elk Horn, IA

Parameter/ Equipment	Attenuation – Source <sup>1</sup>										
Reference Standard, Method, and/or Equipment	Comparison to 8496H Attenuator										
Range	Expanded Uncertainty of Measurement (+/-)										
Frequency Ranges	Step Attenuation Level in dB										
	10	20	30	40	50	60	70	80	90	100	110
1 kHz ≤ f < 100 MHz	0.0037	0.0071	0.052	0.064	0.049	0.089	0.083	0.12	0.14	0.16	0.2
100 MHz ≤ f < 300 MHz	0.0042	0.0092	0.058	0.071	0.055	0.089	0.083	0.12	0.14	0.17	0.18
300 MHz ≤ f < 500 MHz	0.0073	0.014	0.065	0.079	0.062	0.096	0.088	0.13	0.14	0.18	0.19
500 MHz ≤ f < 1 GHz	0.0073	0.016	0.082	0.086	0.071	0.1	0.094	0.13	0.15	0.22	0.24
1 GHz ≤ f < 4 GHz	0.0096	0.02	0.097	0.1	0.086	0.11	0.1	0.15	0.16	0.22	0.24
4 GHz ≤ f < 8 GHz	0.011	0.023	0.1	0.11	0.089	0.15	0.14	0.19	0.21	0.36	0.37
8 GHz ≤ f < 10 GHz	0.016	0.032	0.12	0.13	0.11	0.19	0.18	0.27	0.28	0.42	0.45
10 GHz ≤ f < 12 GHz	0.019	0.039	0.12	0.12	0.1	0.16	0.15	0.2	0.23	0.38	0.46
12 GHz ≤ f < 14 GHz	0.022	0.045	0.14	0.14	0.12	0.2	0.19	0.27	0.29	0.43	0.51
14 GHz ≤ f < 18 GHz	0.032	0.063	0.14	0.14	0.12	0.21	0.2	0.27	0.29	0.36	0.5
18 GHz	0.039	0.075	0.16	0.17	0.14	0.26	0.24	0.34	0.36	0.56	0.58

**Electrical – RF/Microwave**

Elk Horn, IA

Parameter/ Equipment	RF Power Measure										
Reference Standard, Method, and/or Equipment	Comparison to 8487A, 8487D, E9304A-H18 Power Sensors										
Range	Expanded Uncertainty of Measurement (+/-)										
Power Range	Frequency Ranges (uncertainties in dB)										
	9 kHz To 50 MHz	50 MHz to 500 MHz	500 MHz to 1.2 GHz	1.2 GHz to 6.0 GHz	6.0 GHz to 14 GHz	14 GHz to 18 GHz	18 GHz to 26.5 GHz	26.5 GHz to 33 GHz	33 GHz to 40 GHz	40 GHz to 45 GHz	45 GHz to 50 GHz
-70 to -60 dBm	-	0.819	0.819	0.82	0.821	0.822	0.823	0.824	0.830	0.841	0.843

**Electrical – RF/Microwave**

Elk Horn, IA

Parameter/Equipment		RF Power Measure									
Reference Standard, Method, and/or Equipment		Comparison to 8487A, 8487D, E9304A-H18 Power Sensors									
Range		Expanded Uncertainty of Measurement (+/-)									
Power Range	Frequency Ranges (uncertainties in dB)										
	9 kHz To 50 MHz	50 MHz to 500 MHz	500 MHz to 1.2 GHz	1.2 GHz to 6.0 GHz	6.0 GHz to 14 GHz	14 GHz to 18 GHz	18 GHz to 26.5 GHz	26.5 GHz to 33 GHz	33 GHz to 40 GHz	40 GHz to 45 GHz	45 GHz to 50 GHz
-60 to -50 dBm	1.789	0.257	0.257	0.258	0.266	0.269	0.28	0.284	0.313	0.360	0.369
-50 to -40 dBm	0.257	0.092	0.093	0.096	0.117	0.125	0.146	0.155	0.205	0.273	0.285
-40 to -30 dBm	0.145	0.094	0.094	0.97	0.118	0.126	0.147	0.156	0.206	0.274	0.286
-30 to -20 dBm	0.108	0.111	0.111	0.113	0.125	0.131	0.175	0.183	0.226	0.275	0.301
-20 to -10 dBm	0.108	0.086	0.080	0.087	0.092	0.101	0.123	0.140	0.145	0.198	0.218
-10 to 0 dBm	0.108	0.087	0.080	0.088	0.093	0.103	0.127	0.145	0.150	0.207	0.228
0 to 10 dBm	0.099	0.087	0.080	0.088	0.093	0.103	0.127	0.145	0.150	0.207	0.228
10 to 20 dBm	0.096	0.100	0.100	0.097	0.109	0.122	0.160	0.170	0.173	0.252	0.270

**Mass and Mass Related**

Elk Horn, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Barometers	(22 to 34) inHg (750 to 1 150) mBar	0.011 inHg 0.39 mBar	Comparison to DPI 740 Barometer

**Thermodynamic**

Elk Horn, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Relative Humidity	(0 to 90) %RH (90 to 100) %RH	1.3 %RH 2.4 %RH	Comparison to Vaisala hygrometer

**Thermodynamic**

Elk Horn, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Relative Humidity	(5 to 90) %RH (90 to 95) %RH	0.81 %RH 1 %RH	Comparison to Rotronic HG2-S101 Humidity Generator and Rotronic H290D sensor
Temperature	(5 to 60) °C	0.14 °C	Comparison to Rotronics HG2-S101 Humidity Generator and Rotronics H290D sensor
Temperature	(-200 to 0) °C (0 to 200) °C (200 to 660) °C	0.021 °C 0.022 °C 0.027 °C	Comparison to Fluke 5618B, 5628B RTD Probes and 1523 Temperature Indicator
Temperature	(-70 to 0) °C (0 to 180) °C	0.021 °C 0.022 °C	Comparison to Fluke 5628B RTD Probe and 1523 Temperature Indicator, comparison to reference thermometer, in temperature chambers

**Time and Frequency**

Elk Horn, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Frequency – Measuring Equipment	1 mHz to 80 MHz	2.5 μHz/Hz + 1 μHz	Comparison to Agilent 33250 Signal Generator with GPS conditioning
Frequency – Measuring Equipment	10 Hz to 4 GHz	0.03 nHz/Hz + 0.6 mHz	Comparison to Fluke 9640 Reference Source with GPS conditioning
Frequency – Measuring Equipment	10 MHz to 50 GHz	0.03 nHz/Hz + 0.6 Hz	Comparison to Agilent 83650B w/ option 008 Signal Generator with GPS conditioning
Frequency – Measuring Equipment 10 MHz Source (Rubidium)	10 MHz	0.03 nHz/Hz	Comparison to Rubidium frequency standard referenced to GPS

**Time and Frequency**

Elk Horn, IA

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Frequency – Measure	1 Hz to 225 MHz 225 MHz to 50 GHz	0.06 nHz/Hz + 25 pHz 0.04 nHz/Hz + 2 Hz	Comparison to Agilent 5335A, 53132A, Agilent 53151A, 53132A Counters, 8565E Spectrum Analyzer with GPS conditioning
Frequency – Measure	10 MHz	0.003 nHz/Hz	Comparison to Agilent 53132A Counter referenced to GPS
Time Interval – Measure	120 ps to 400 s	19 μs/s + 24 ps	Comparison to Tektronix TDS 7404B oscilloscope
Time Interval – Measure	(1 to 3 600) s	0.008 8 s	Comparison to Agilent 33250A Signal Generator, with photo comparison

[Return to Site listing \(top\)](#)

Calibration and Measurement Capability (CMC) is expressed in terms of the measurement parameter, measurement range, expanded uncertainty of measurement and reference standard, method, and/or equipment. The expanded uncertainty of measurement is expressed as the standard uncertainty of the measurement multiplied by a coverage factor of 2 ( $k=2$ ), corresponding to a confidence level of approximately 95%.

- Notes:
- Unitless linear measure.
  - Capability only available in Malaysia.
  - $D$  = diameter in inches,  $f$  = frequency,  $L$  = length in inches,  $M$  = modulation rate,  $P$  = power applied,  $R$  = resolution of device under test, “ $p$ ” = modulation accuracy or rho,  $S$  = step (dB),  $T$  = Temperature in °C,  $\tau$  = applied torque lbf in.
  - The CMC for scales and balances is highly dependent upon the resolution of the unit under test. The uncertainties presented here do not include the resolution of the unit under test. The resolution will be included in the reported measurement uncertainty at the time of calibration.



Jason Stine, Vice President